

Rapid Sample Preparation and Analysis of 107 Pesticides in Water with the Solid Phase Extraction Disk Cartridge and Gas Chromatography Mass Spectrometer

Reika Takahara, Takumi Kunieda, Kazuyuki Ishi, Manabu Takayanagi, Hiroshi Hayashida
GL Sciences Inc., Tokyo, Japan

Introduction

Gas chromatography mass spectrometer (GC-MS) and liquid chromatography mass spectrometer (LC-MS) are generally used for pesticide analysis in water, while solid phase extraction (SPE), which is easier to automate and uses less solvent, is preferred as a sample concentration method. SPE may concentrate analytes hundreds of times their concentration in the sample, allowing for the detection of analytes with very low concentrations. Conversely, SPE operation is complex, requiring conditioning of the SPE cartridge, sample application, washing, dehydration, elution, and distillation of the evaporation solvent as needed, and taking several hours for each preparation. If the number of samples is enormous, it may take up to an hour to apply the SPE cartridge. In this study, we report that the time for SPE in the analysis of 107 pesticides in water was greatly reduced using the new shape of SPE cartridge "EZ cartridge RP-1". The EZ cartridge RP-1 has an SPE membrane fixed in a polypropylene housing. This membrane is composed of reversed-phase mode divinylbenzene - methacrylate copolymer particles and polytetrafluoroethylene (PTFE) fibered and is molded to a diameter of 25 mm and a thickness of 0.5 mm. Because of its large cross-sectional area, water sample passage at the same linear speed can theoretically be increased by approximately five times compared to a typical SPE cartridge. Due to the diameter of the solid phase particle being only 10 μm , it is possible to strongly retain an analyte, preventing the analyte from breaking through.

Methods

Solutions and mixtures for sample preparation were extracted and analyzed as shown in Table 3. The standard sample was prepared by diluting a pesticide standard mixture (Hayashi Pure Chemical Ind., Ltd.) and adding it to the sample water. The SPE cartridge, EZ Cartridge RP-1 (GL Sciences, Inc.), is filled with a reverse mode SPE membrane made of methacrylate divinylbenzene copolymer. The 500 mL sample was concentrated to 0.5 mL before being adjusted to 1 mL with dichloromethane. The entire procedure, from conditioning the SPE cartridge, to elution with dichloromethane, was performed automatically by the Aqua Trace ASPE899 (GL Sciences, Inc.). The GCMS-QP2020 NX was used to examine the material (Shimadzu). The internal standard was a mixture of Anthracene-d10, Chrysene-d12, and 9-Bromoanthracene, with 9-Bromoanthracene for correction. The InertCap 5MS/Sil capillary column was employed, which is a low-polar column having a liquid phase of 5% diphenyl (equiv.) - 95% dimethyl silphenylene siloxane.

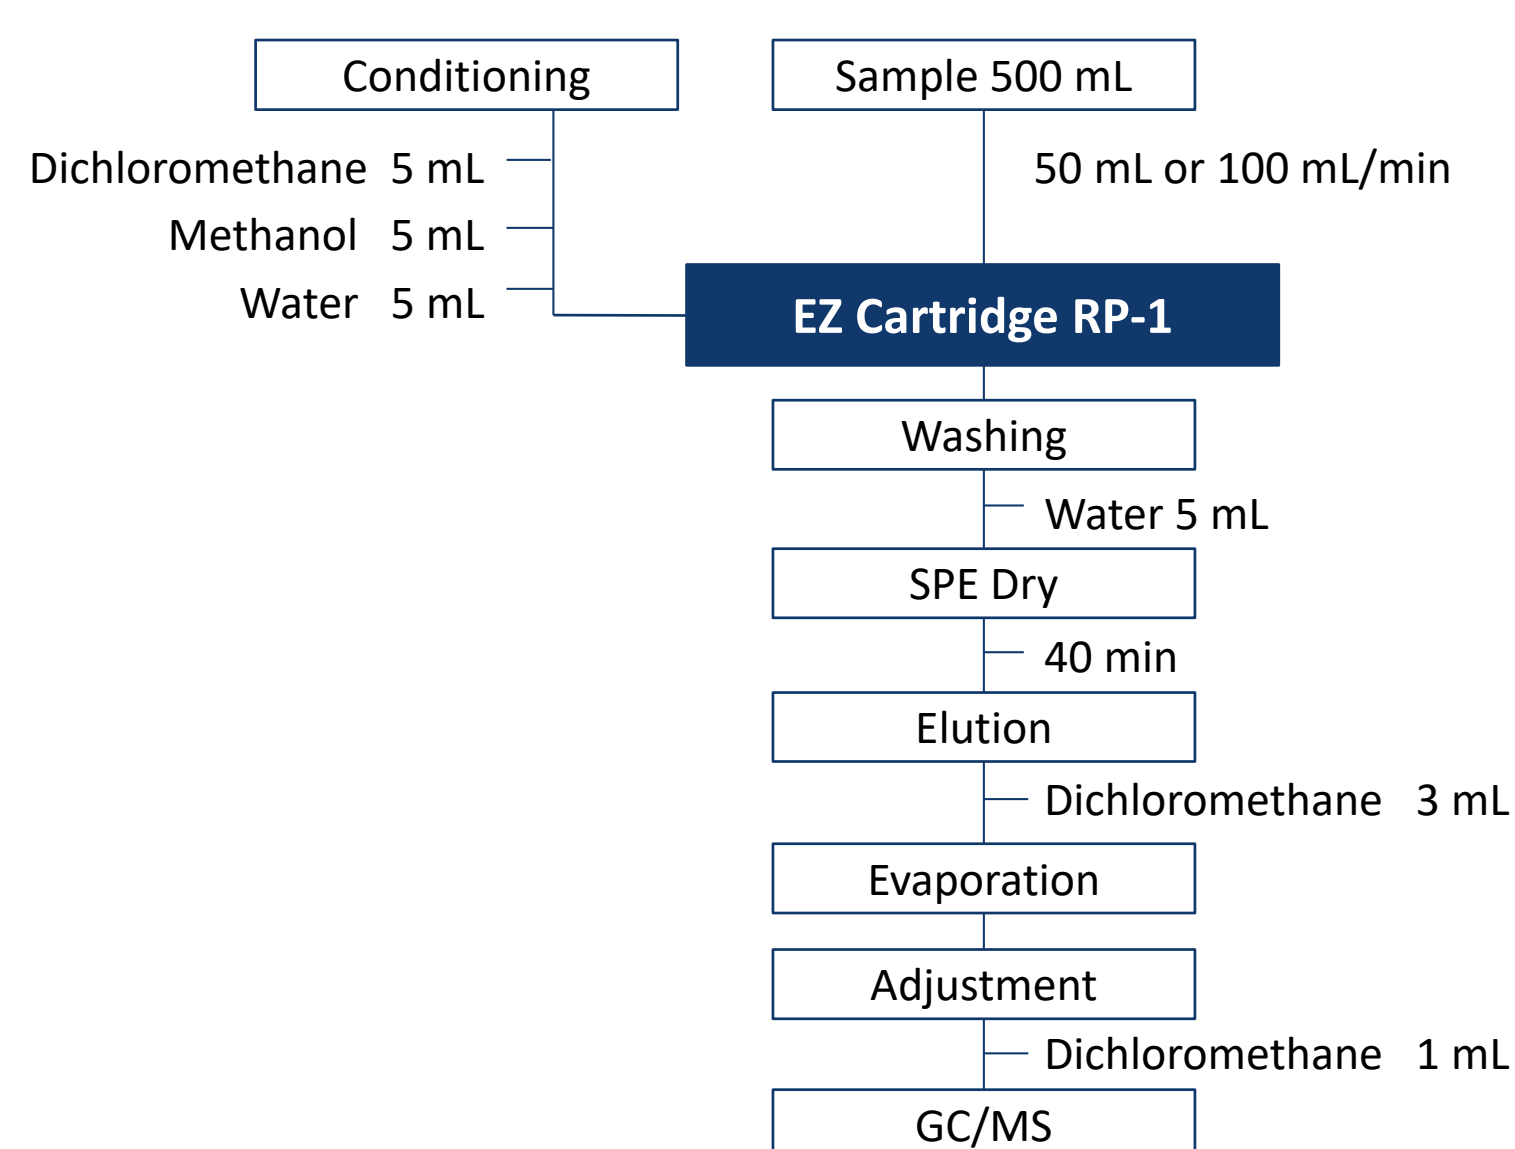



Fig.1 Solid Phase Extraction Procedure

Table 1 Comparison of SPE cartridge structure and sample flow rate

	EZ Cartridge	Conventional SPE Cartridge
Structure		
Particle size and diffusion efficiency	10 μm	60 - 70 μm
Sample Volume	500 mL	500 mL
Flow Rate	100 mL/min	10 mL/min
Time	5 min	50 min
Relationship between liner velocity and sample passage area		

Results

Pesticides in water were concentrated from 500 mL to 1 mL using an EZ cartridge RP-1 and analyzed using GC-MS. As shown in Table 3, the EZ cartridge had a good recovery rate. The number of pesticides with a recovery rate of 70% or higher in 107 cartridges was 101 components when the sample was passed at 50 mL/min and 104 components when the sample was passed at 100 mL/min.

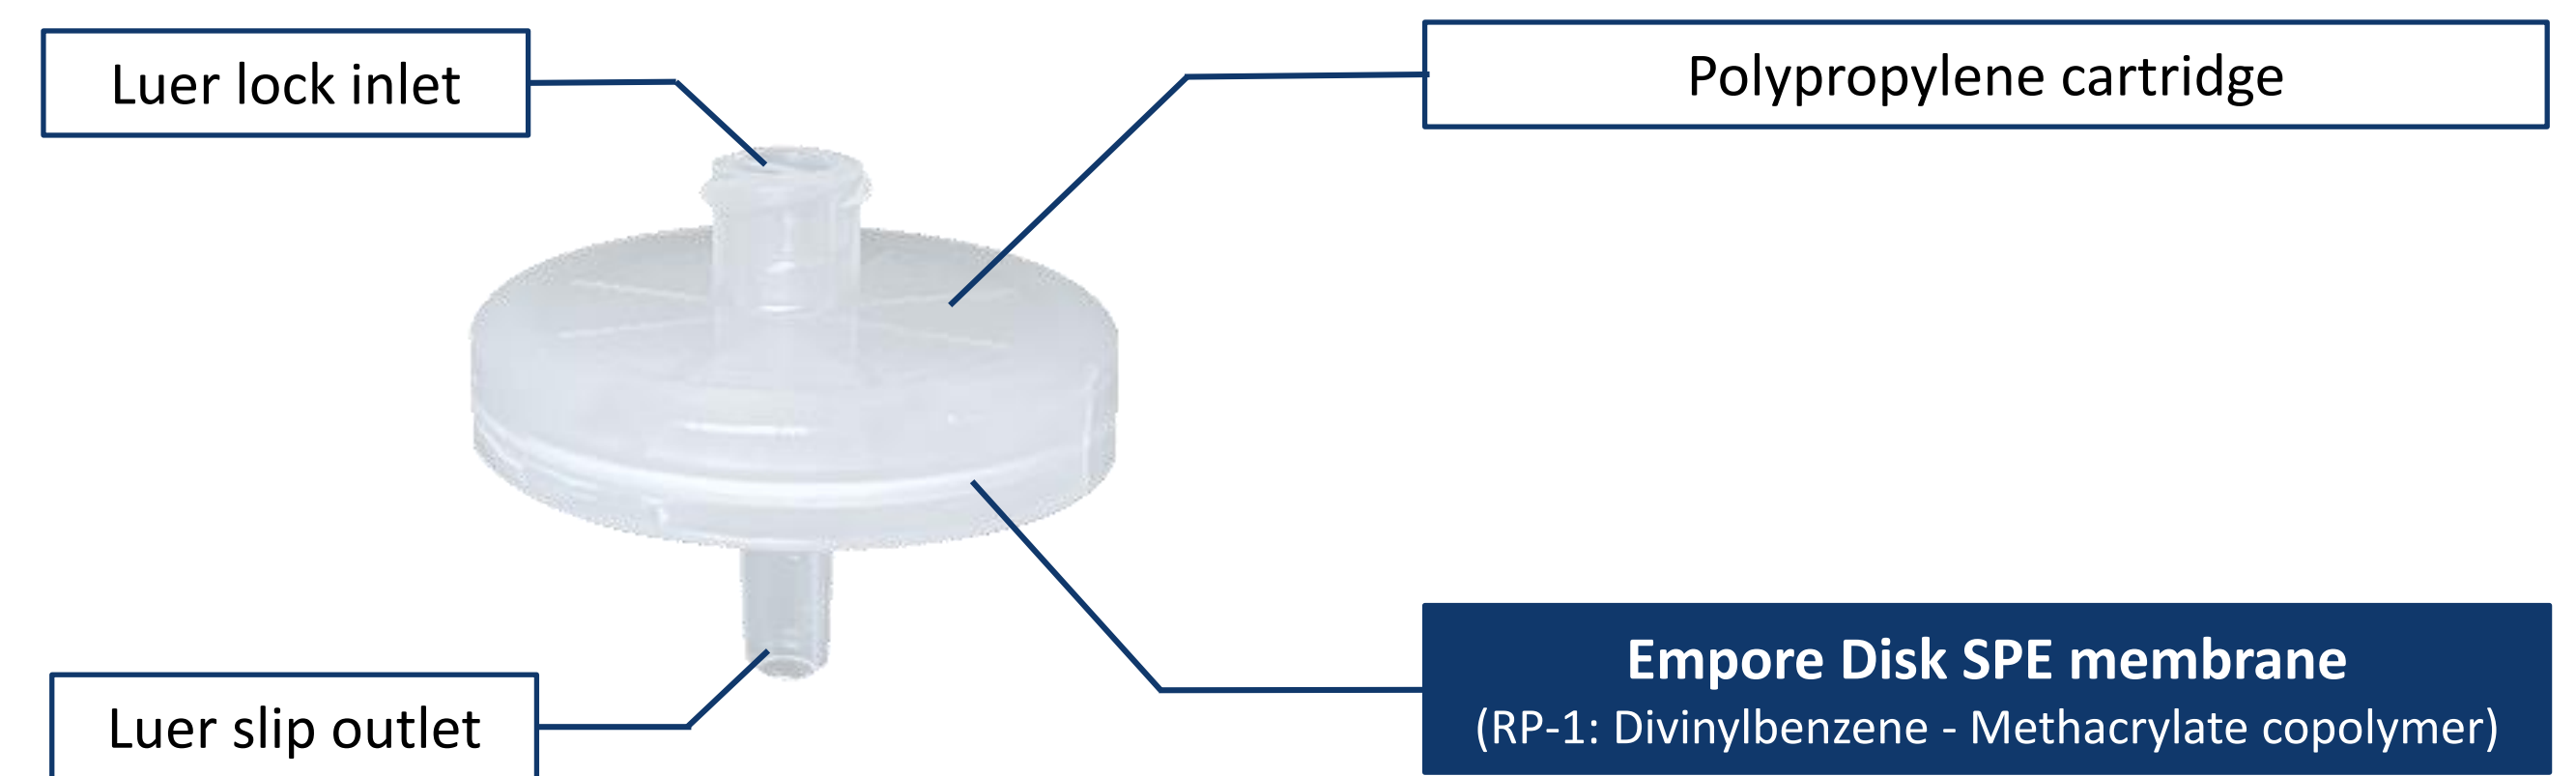

EZ Cartridge RP-1
Solid Phase Extraction Disk Cartridge

Table 2 GC-MS Conditions

System	GCMS-QP2020 NX (Shimadzu)
Column	InertCap 5MS/Sil (GL Sciences Inc.) 0.25 mm I.D. × 30 m df = 0.25 μm
Col. Temp.	50 °C (3 min hold) - 10 °C/min - 200 °C - 3 °C/min - 230 °C (5 min hold) - 5 °C/min - 280 °C (2 min hold)
Carrier Gas	He, 100 kPa
Injection	Splitless, 1min, 250 °C
Detection	MS SIM
Interface Temp.	280 °C
Sample Size	1.0 μL

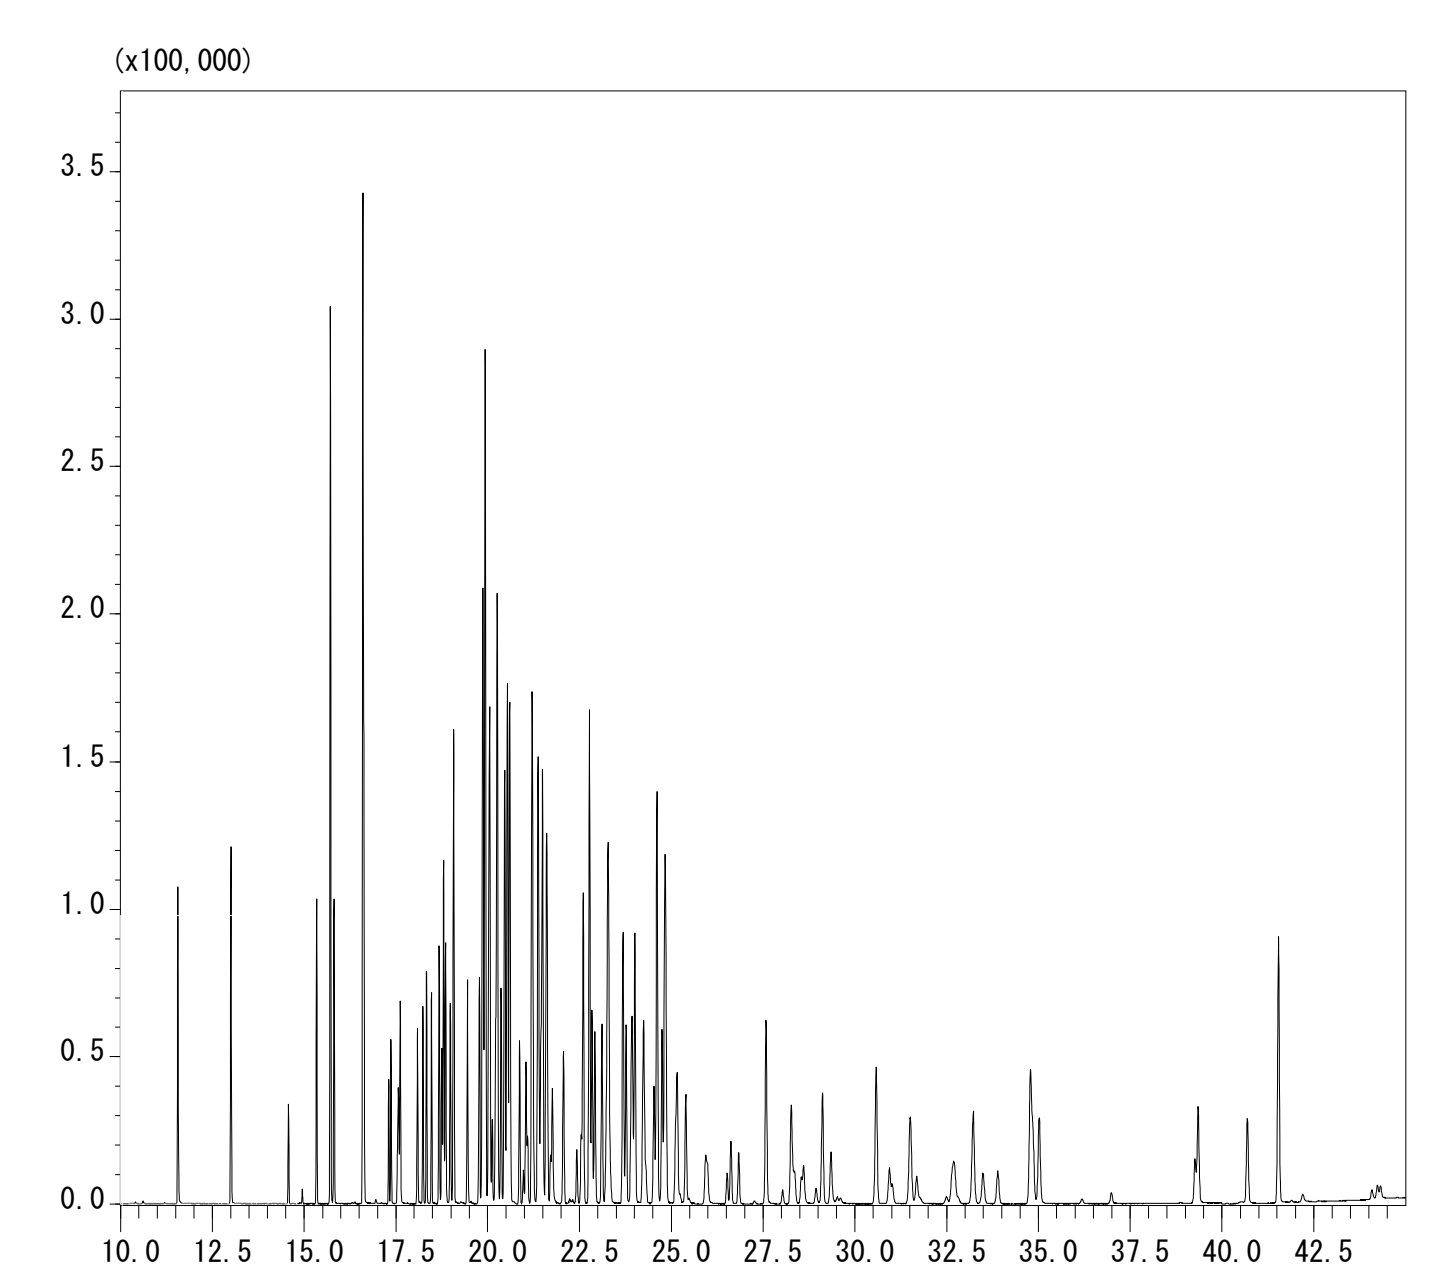


Fig.2 Total Ion Current Chromatogram

Table 3 Repeatability Linearity, and Recovery

NO.	Compounds	100 mL/min		50 mL/min		NO.	Compounds	100 mL/min		50 mL/min	
		Recovery Rate (%)	CV (% n = 3)	Recovery Rate (%)	CV (% n = 3)			Recovery Rate (%)	CV (% n = 3)		
1	Dichlorvos	75.8	9.6	76.3	2.8	55	Phenthoate	77.4	6.7	73.6	5.2
2	Etridiazole	65.9	11	70.4	4.3	56	Captan	78.7	3.4	78.4	2.2
3	Chloroneb	81.1	10.5	81.8	1.9	57	Procyimazole	85.4	4.9	81.4	2.3
4	Isoprocarb	81.1	8.4	78.6	2.6	58	Dimepiperate	77.6	5.6	76.4	4.5
5	Fenobucarb	82	7.8	79.1	2.6	59	Butamifos Oxon	75.2	8.5	74.3	7.2
6	Propoxur (PHC)	77.9	4.2	80.3	3.2	60	Methidathion	84.7	4.8	77.1	4.8
7	Pecycuron	86.1	8.1	78.3	5.5	61	Propaphos	75.5	6.8	73.1	5.7
8	Simazine	83.5	4.9	67.6	4.6	62	Tetrachlorvinphos (CVMP)	78.2	5	79.1	5.8
9	Atrazine	83.4	5	77.8	4.4	63	Paclobutrazol	81.6	6.4	76.8	5.3
10	Diazinon Oxon	82.3	5.9	76.2	6.6	64	Butachlor	75	6.5	75	4.9
11	Cyanophos (CYAP)	74.7	6.4	74.7	4.1	65	alpha-Endosulfan	73.1	5.5	77.7	2.4
12	Propryzamide	85.3	5.6	76	4.9	I.S.2	9-Bromoanthracene	-	-	-	-
13	Diazinon	77.3	7.8	73.7	4.3	66	Butamifos	78.4	5.3	74.9	6.3
14	Pyroquilon	79.1	6.8	78.8	2.8	67	Napropamide	87.3	6.3	79.1	4.6
15	Chlorothalonil (TPN)	75.2	4.3	71.7	3.9	68	Flutolanil	88.9	5.4	80.1	5.6
16	Anthracene-d10	-	-	-	-	69	(E)-Metominostrubin	83.7	6.2	79.9	5.7
17	Ethylthiomethon	74.9	8.1	74.9	3.6	70	Pretlialchlor	84.6	6	77.4	4.4
18	Iprobenfos	78.8	6	76.4	5	71	Isoprothiolane	86.7	5.1	81.5	2.8
19	Tolclofos-methyl Oxon	83	5.2	78.4	4.5	72	Isoxathion Oxon	85.5	5.6	67.4	1.9
20	Benfuresate	79	6.5	77.6	3.7	73	Uniconazole P	80.3	7.3	74.1	5.2
21	MEP Oxon	81	6	80.5	4.9	74	Thifluzamide	80.5	5.9	75.8	5.7
22	Terbutcarb	83.3	5.8	78	5.4	75	MPP Oxon Sulfoxide	81.3	5.3	91.6	4.2
23	Propanil (DCPA)	84.6	5.3	82.4	4.1	76	MPP Oxon Sulfone	80.9	12.8	81.9	6.1
24	Bromobutide	80.6	4.8	75.5	6.6	77	Buprofezin	77.4	6.1	77.4	3.2
25	Metribuzin	78.6	4.3	77.4	5.3	78	Cyproconazole	78.1	8.4	73.4	6
26	Malaon	88.4	11.8	91.9	7.3	79	(Z)-Pyriminobac-methyl	80.5	7.1	74.8	4.8
27	Simeconazole	78.8	5.1	76.2	5.9	80	MPP sulfoxide	78.6	5.1	78.9	3.3
28	Alachlor	82.5	5.6	77.7	4.2	81	beta-Endosulfan	73.7	5.4	78	2.8
29	Simetryne	77.9	4.5	69.3	6.3	82	MPP sulfone	78.7	5.7	78.4	5.4
30	Metaxyl	84.2	6.6	80.2	4.6	83	Meprotil	88.5	6.5	79.3	4.4
31	Ametryn	79.5	5.7	75.7	5.1	84	Chlornitrofen (CNP)	68.2	8.9	76.6	6.4
32	Cinmethylin	76.6	5.9	78.4	3.5	85	Edifenphos	87.7	4.8	79.2	5.8
33	MPP Oxon	79.8	4.4	79.9	6.1	86	Propiconazole1	85.1	6.1	74.9	7.3
34	Fenitrothion	81.4	4.9	77.2	5.5	87	Endosulfate	69.8	3.4	81.8	8.6
35	Bromacil	79.6	5.7	78.8	7	88	(E)-Pyriminobac-methyl	80.2	6.1	71.2	6.8
36	(E)-Dimethylvinphos	82.2	5.2	82.7	7.3	89	Propiconazole2	82.8	7.1	72.6	6.4
37	Espocarb	79.5	6.9	78.5	3.2	90	EPN Oxon	84.2	9.8	81.1	7.3
38	Malathion	85.9	4.8	79.6	5.3	91	Thenylchlor	87.3	5.2	78.1	6.6
39	Chlorpyrifos Oxon	86.9	7.2	81	6.7	92	Tebuconazole	80	7.2	76.7	4.6
40	Quinoclamine (ACN)	74.2	4.4	76.7	4.5	93	Pyridaphenthion	79	8	69.5	8.2
41	Metolachlor	78.2	5.8	75.4	4.9	94	Acetamidid	70.4	6	70.6	7.8
42	Thiobencarb	81.8	5.9	79.3	1.8	95	Iprodion	79.3	5.2	74.5	6.8
43	(Z)-Dimethylvinphos	79.6	3.9	79.2	3.5	I.S.3	Chrysene-d12	-	-	-	-
44	Cyanazine	78.8	3.4	79.4	3.9	96	EPN	73	9.4	77.9	6.9
45	Fenthion	79.9	5.8	77.5	3.3	97	Piperophos	71.7	10.1	66	7.8
46	Chlorthal-dimethyl (TCTP)	73.2	4.6	76.9	2	98	Indanofan	72.3	11.5	29.6	6.4
47	Isofenphos Oxon	83.2	8.8	76.3	7.7	99	Furametpyr	79	6.7	73	7.2
48	Tetraconazole	76.9	5	73.6	5.9	100	Iprodion metabolite	71.5	7.2	74.3	5.2
49	Fthalide	81.5	4	79.1	2.7	101	Mefenacet	79.2	6.4	74.7	6.9
50	Fosthiazate	83.2	6.3	89.9	3.7	102	CNP-amino	87.1	5.4	78.4	4.4
51	Cyprodinil	75.2	5.2	74.3	3.8	103	Etobenzanid	84.4	8	78.1	5.7
52	Dimethametryn	80	6.2	72.5	5.8	104	Cafenazole	91.7	6	83.2	4.8
53	Isofenphos	79.6	5.1	76.4	4.3	105	Boscalid	87.2	6.2	77.5	4.5
54	Methidymron	80.2	4.5	77.9	3.5	106	Thiocluprid	80.7	4.7	81.8	6.2
						107	Pyrazoxyfen	81.5	6.4	79.9	4.2

Conclusions

Using an EZ cartridge in the sample preparation for pesticide analysis in water, it was possible to reduce the time required for solid phase extraction from 162 min to 80 min. The EZ cartridge RP-1 is packed with reversed-phase polymers and is highly versatile; thus, it is likely to be applied with hydrophobic chemical compounds other than pesticides.

References

- Standard test method in water, Ministry of Health, Labor and Welfare, Japan
- Water Supply Test Method 2011 Edition, Japan Water Works Association