


InertSearch™ for GC

InertCap® Applications

D-glucose-TMS

Data No. GA018-0000

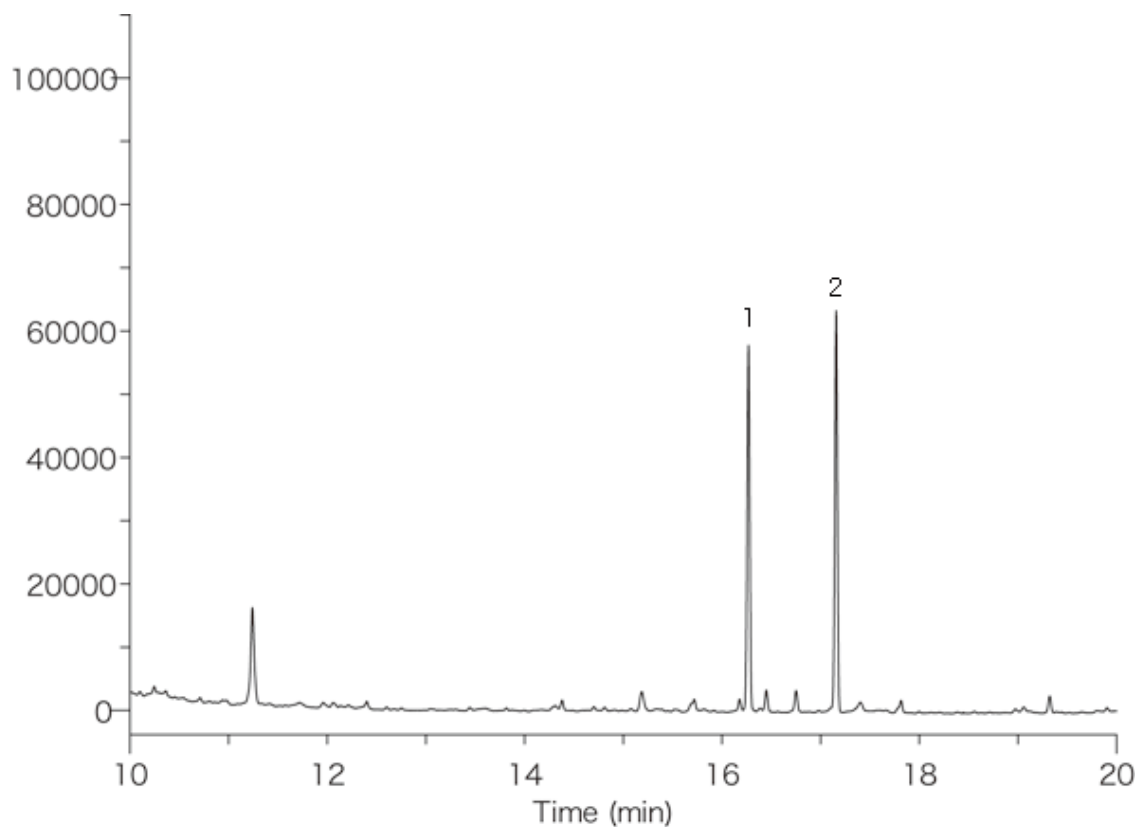

System : GC/FID
Column : InertCap 1
0.25mm I.D. × 30m df=0.25µm
Column Temp. : 100°C (2min) → 10°C/min → 300°C
Carrier Gas : He 80kPa
Detection : FID
Sample : D-glucose-TMS

Solutes : 1. α-D-glucose-TMS
2. β-D-glucose-TMS