


Organic solvents

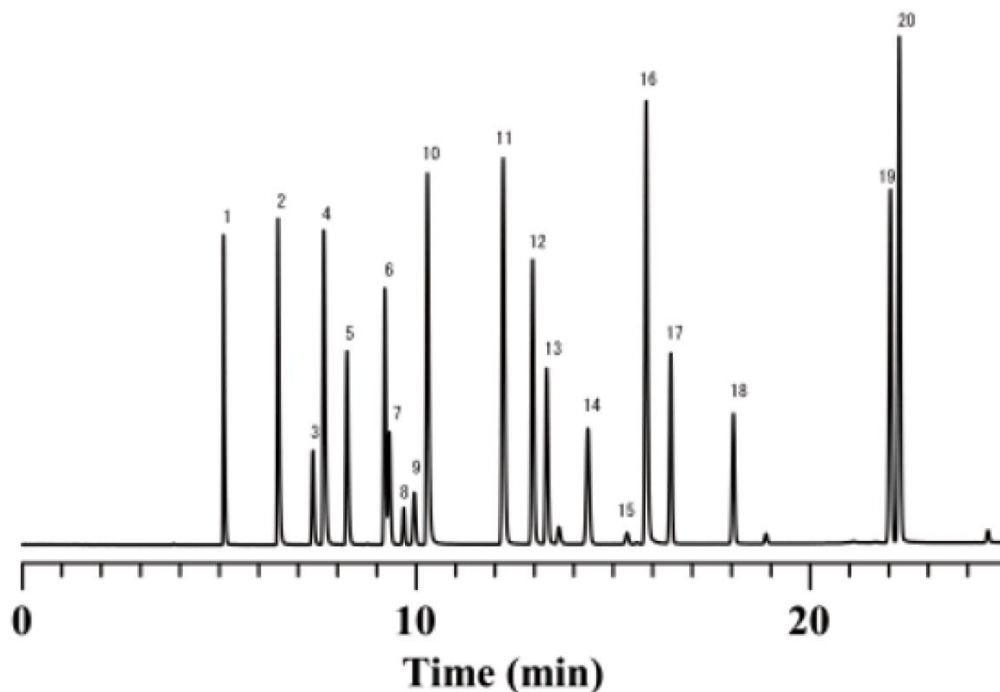

System : GC/FID
 Column : InertCap AQUATIC-2
 0.25 mmI.D. × 60 m df=1.4 μm
 Column Temp. : 40 °C(min)→4 °C/min→120 °C→10 °C/min→250 °C
 Carrier Gas : He 200 kPa
 Injection : Split 1 : 80 1μL
 Detection : FID

Solutes : 1. Methanol
 2. Ethanol
 3. Diethylether
 4. 2-Propanol
 5. Acetone
 6. Acetonitrile
 7. Methylacetate
 8. Dichloromethane
 9. n-Hexane
 10. n-Propanol
 11. MEK
 12. 1,2-Dichloropropane
 13. Ethylacetate
 14. Cyclohexane
 15. Carbontetrachloride
 16. 1-Butanol
 17. 1,2-Dichloroethane
 18. Trichloroethylene
 19. iso-Butylacetate
 20. Toluene