


Organic solvents

Data No. GA035-0000

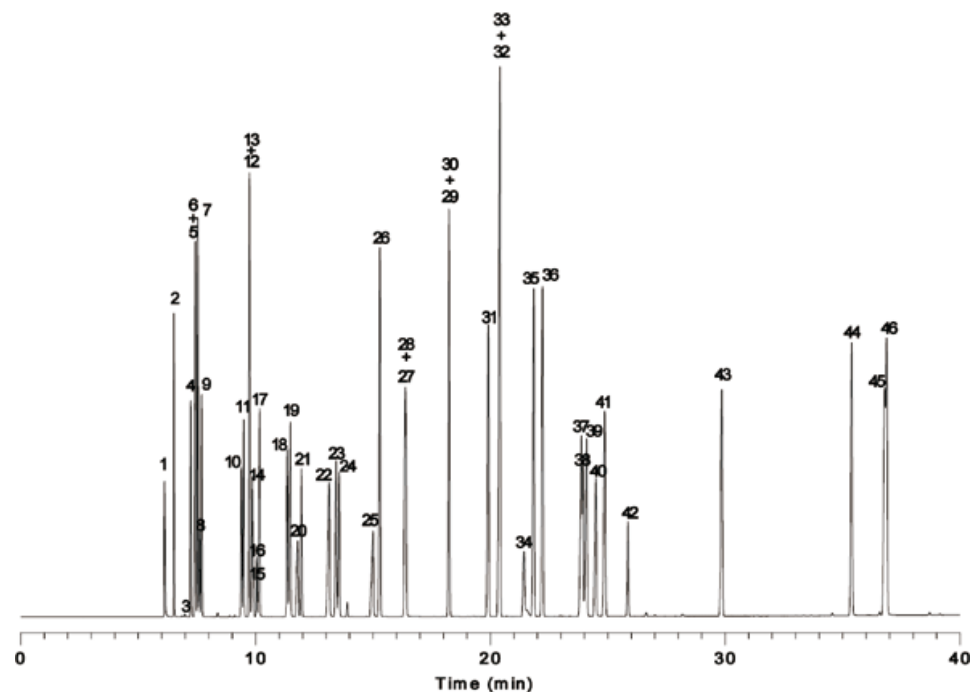

System	: GC/FID	Solutes :	1. Methanol	26. Toluene
Column	: InertCap 1701 0.25mm I.D.×60m df=0.25µm		2. Ethyl ether	27. Tetrachloroethylene
Column Temp.	: 40°C (5min)→4°C/min →230°C (5min)		3. Carbon disulfide	28. i-Amyl alcohol
Carrier Gas	: He 130kPa		4. Acetone	29. Methyl-n-butyl ketone
Injection	: Split 100mL/min 1µL 250°C		5. i-Propanol	30. n-Butyl acetate
Detection	: FID Range 10 ¹ 250°C		6. Methyl acetate	31. Chlorobenzene
Sample	: Organic solvents Mixed evenly		7. n-Hexane	32. m-Xylene
			8. Dichloromethane	33. p-Xylene
			9. trans-1,2-Dichloroethylene	34. N,N-Dimethyl formamide
			10. cis-1,2-Dichloroethylene	35. o-Xylene
			11. Ethyl acetate	36. Styrene
			12. Tetrahydrofuran	37. 1-Methylcyclohexanol
			13. Methyl ethyl keton	38. Cellosolve acetate
			14. 1,1,1-Trichloroethane	39. Cyclohexanol
			15. Carbon Tetrachloride	40. Butyl cellosolve
			16. Chloroform	41. Cyclohexanone
			17. 2-Butanol	42. 1,1,2,2-Tetrachloroethane
			18. 1,2-Dichloroethane	43. o-Dichlorobenzene
			19. i-Butanol	44. o-Cresol
			20. Methyl cellosolve	45. m-Cresol
			21. Trichloroethylene	46. p-Cresol
			22. n-Butanol	
			23. n-Propyl acetate	
			24. 1,4-Dioxane	
			25. Ethyl cellosolve	