


# Free fatty acids

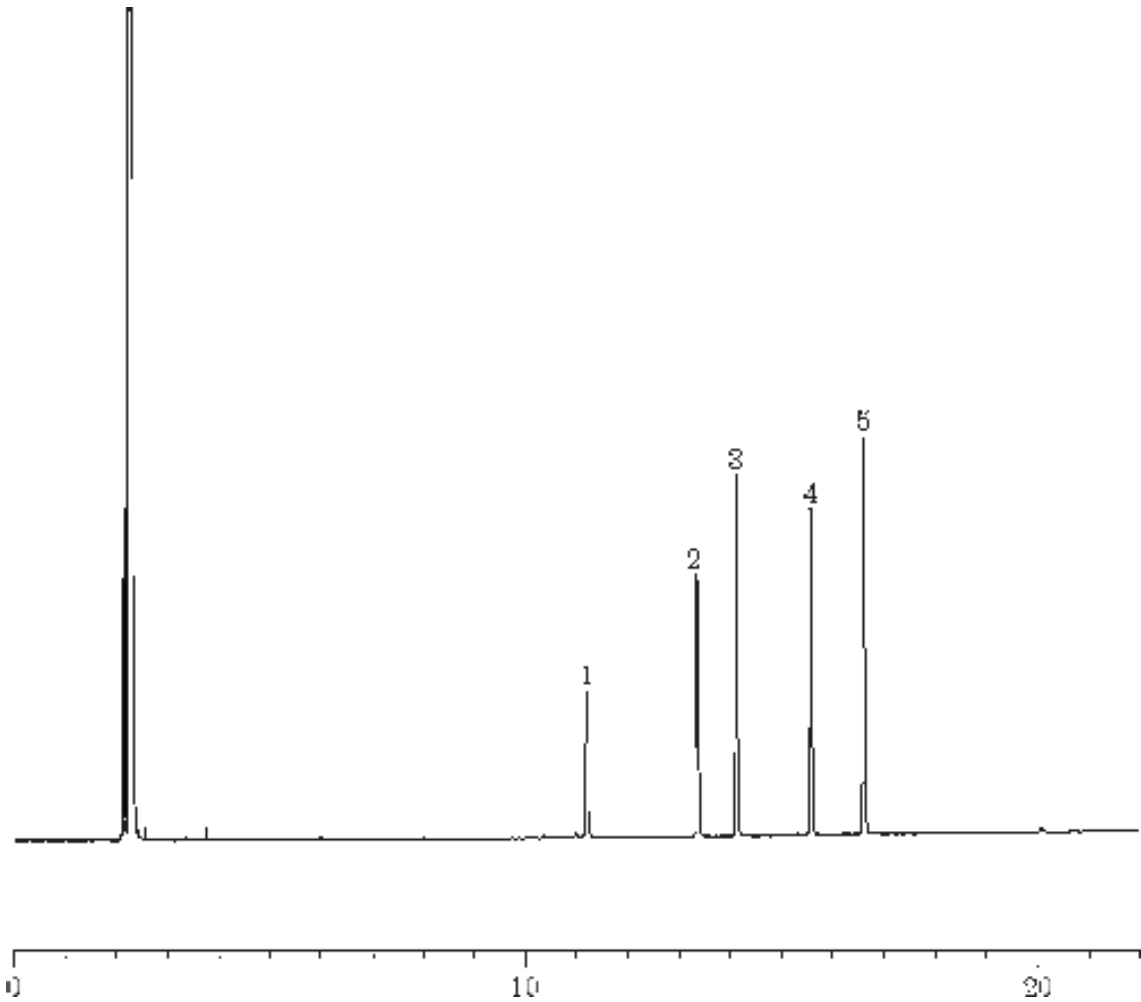

System : GC/FID  
 Column : InertCap Pure-WAX  
 0.25mmI.D. × 30m df=0.25µm  
 Column Temp. : 60°C→5°C/min→200°C  
 Carrier Gas : He 100kPa  
 Injection : Split 1:50 0.1µl  
 250°C  
 Detection : FID Range 10<sup>0</sup>  
 260°C  
 Sample : Fatty acid  
 0.1% Solvent: Cyclohexane

Solutes : 1. Acetic acid  
 2. Propionic acid  
 3. iso-Butyric acid  
 4. Butyric acid  
 5. iso-Valeric acid