


Organic solvents

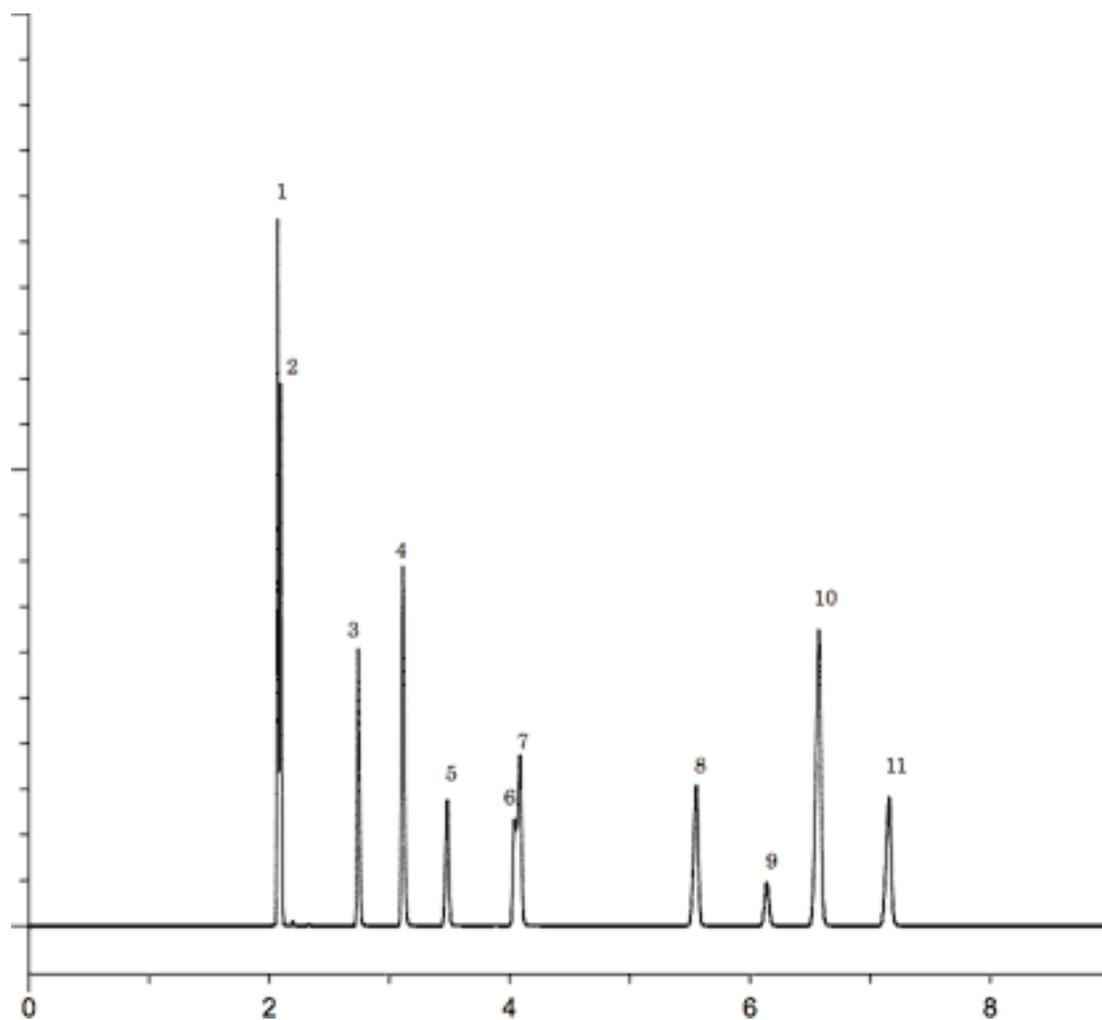

System : GC/FID
 Column : InertCap Pure-WAX
 0.25mmI.D. × 30m df=0.25µm
 Column Temp. : 40°C(5min)→5°C/min→200°C
 Carrier Gas : He 100kPa
 Injection : Split 1 : 80 0.1µl
 250°C
 Detection : FID Range 10⁰
 260°C
 Sample : Organic solents

Solutes : 1. n-Hexane
 2. Diethylether
 3. Acetone
 4. Tetrahydrofuran
 5. Methanol
 6. Dichloromethane
 7. Ethanol
 8. Acetonitrile
 9. Chloroform
 10. Toluene
 11. 1.4-Dioxane