


Isothiocyanate

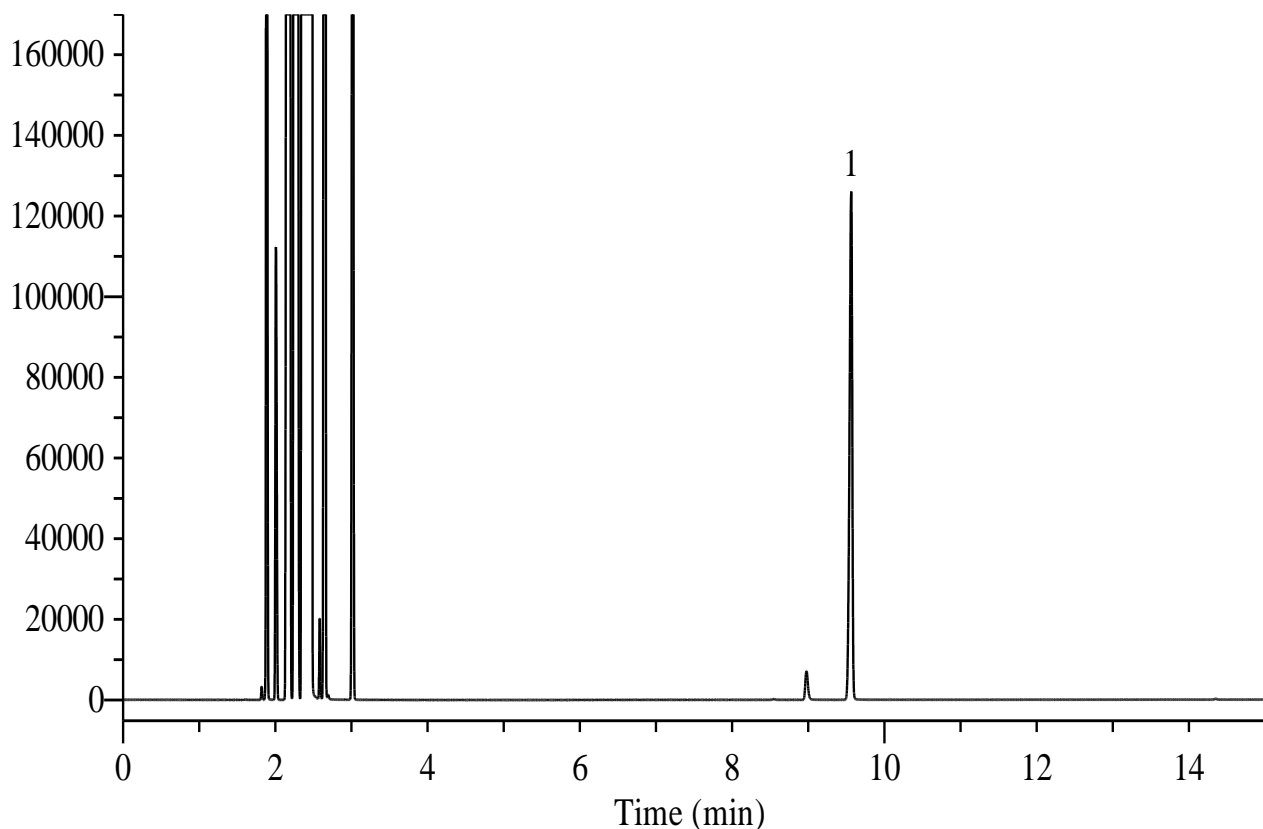

Conditions

System : GC/FID
Column : InertCap 5
 0.25 mm I.D. x 30 m df = 0.25 µm
Col. Cat. No. : 1010-18142
Col. Temp. : 40 °C (5 min hold) - 5 °C/min - 200 °C
Carrier Gas : He 100 kPa
Injection : Split flow 67 mL/min
 200 °C
Detection : FID Range 10⁰
 200 °C
Sample Size : 1000 µg/mL in Hexane
 1 µL

Analyte : 1. Allyl isothiocyanate

