
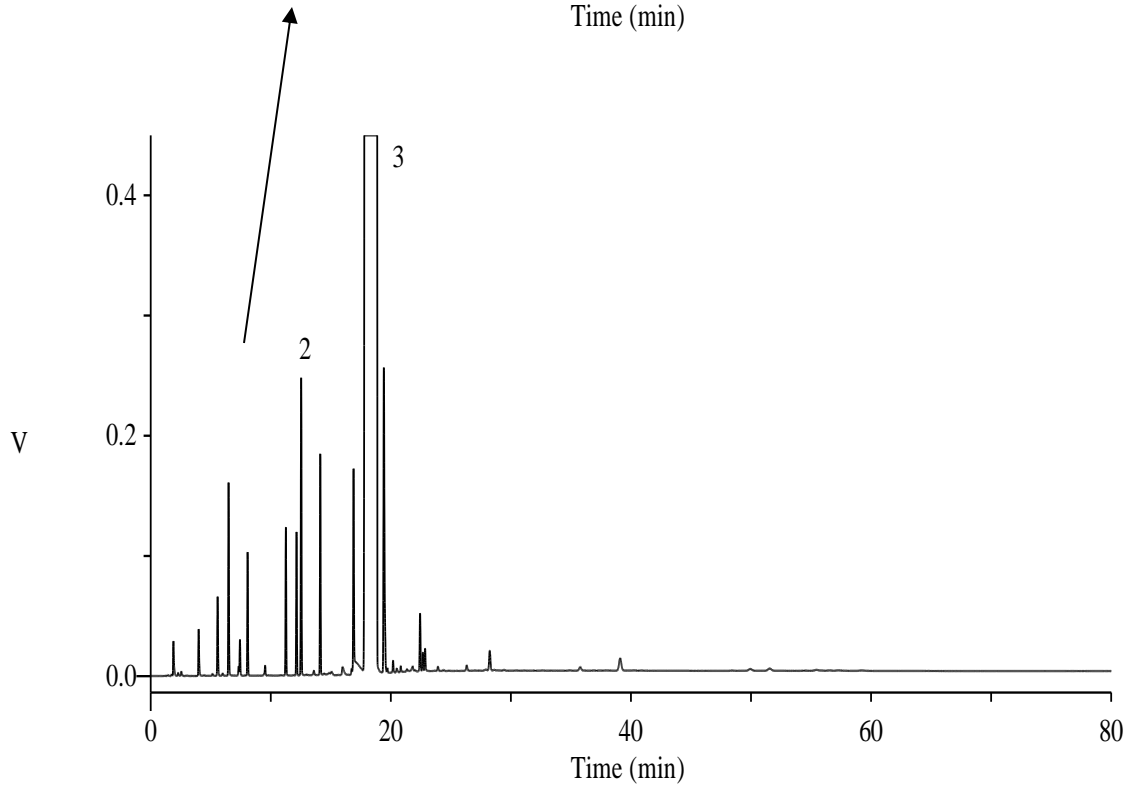


Impurities in Triethylene glycol

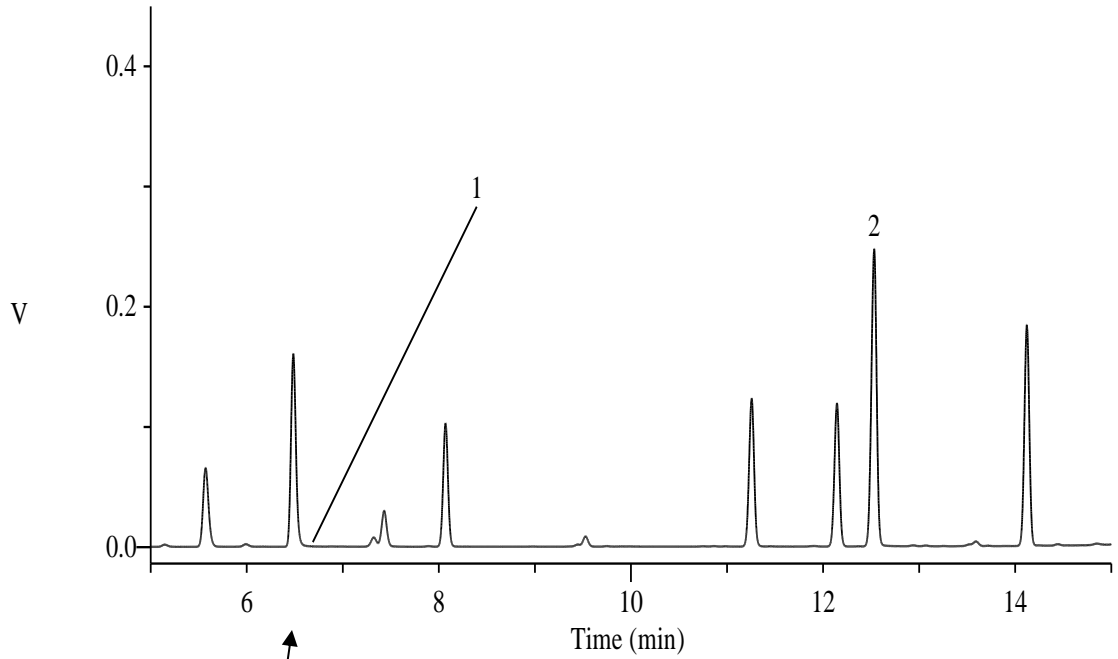

Impurities in Triethylene glycol


Conditions

System	: GC/FID
Column	: InertCap 1 0.32 mm I.D. x 30 m df = 5.00 μm
Col. Cat. No.	: 1010-11249
Col. Temp.	: 40 °C - 10 °C/min - 250 °C (59 min hold)
Carrier Gas	: He 100 kPa
Injection	: Split flow 40 mL/min 250 °C
Detection	: FID Range 10 ⁰ 250 °C
Sample Size	: Triethylene glycol 1.0 μL


Analyte

1. Ethylene glycol (Nondetection)
2. Diethylene glycol
3. Triethylene glycol


Chemical Structure



1. Ethylene glycol



2. Diethylene glycol



3. Triethylene glycol