


Organic Solvents

Data No. GA 284-0644

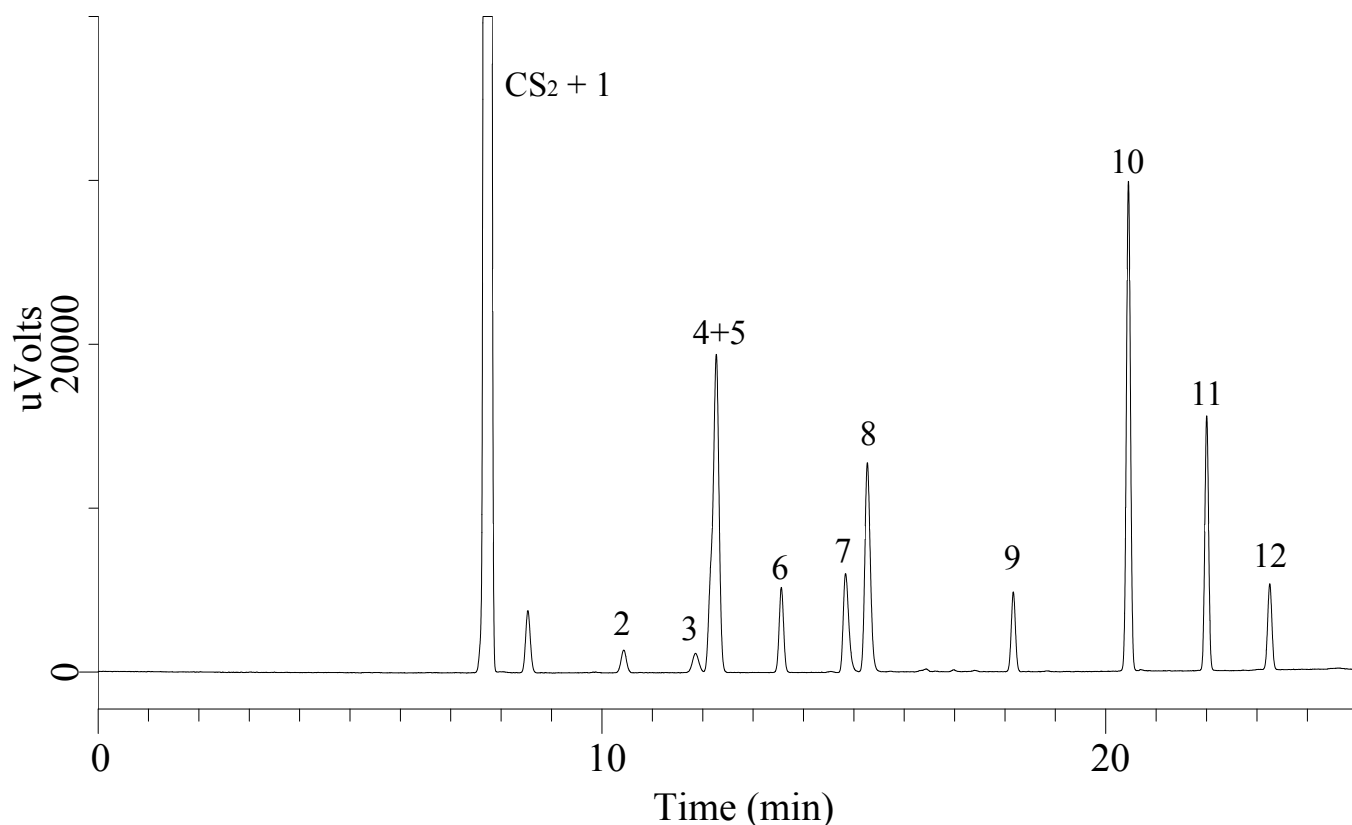

Conditions

System	: GC-FID	Analyte	: 1. Dichloromethane
Column	: InertCap AQUATIC 0.53 mm I.D. x 75 m df = 2.0 µm		2. Chloroform
Col. Cat. No.	: 1010-29477		3. Carbon tetrachloride
Col. Temp.	: 40 °C (5 min hold) - 5 °C/min - 180 °C		4. Benzene
Carrier Gas	: He 5 mL/min		5. 1,2-Dichloroethane
Injection	: Split flow 50 mL/min 220 °C		6. Trichloroethylene
Detection	: FID Auto Range 220 °C		7. 1,4-Dioxane
Sample Size	: 100 µg/mL in Carbon disulfide 1.0 µL		8. 4-Methyl-2-pentanone(MIBK)
			9. Tetrachloroethylene
			10. Ethylbenzene
			11. Styrene
			12. 1,1,2,2-Tetrachloroethane