


Organic Solvents

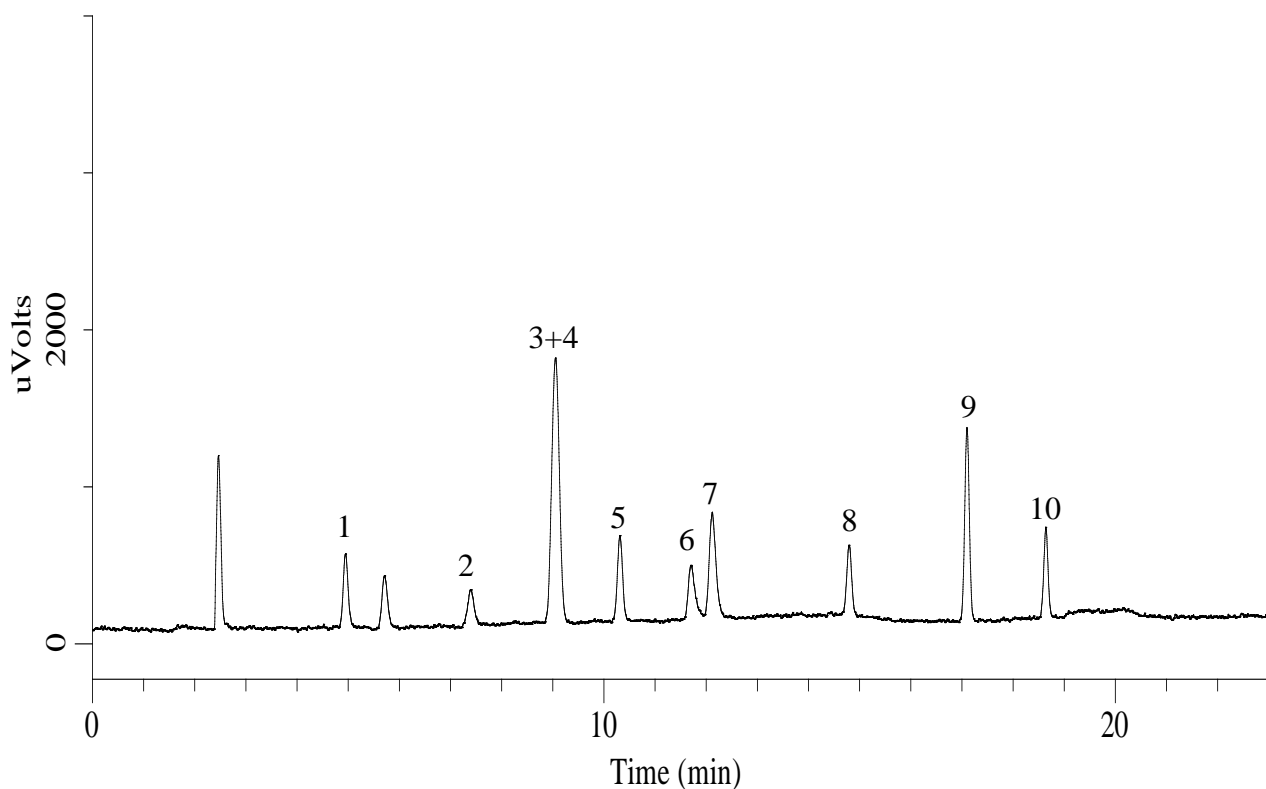

Conditions

System	: GC-FID	Analyte	: 1. Dichloromethane
Column	: InertCap AQUATIC 0.53 mm I.D. x 75 m df = 2.0 μ m		2. Chloroform
Col. Cat. No.	: 1010-29477		3. Benzene
Col. Temp.	: 40 °C (5 min hold) - 5 °C/min - 180 °C		4. 1,2-Dichloroethane
Carrier Gas	: He 10 mL/min		5. Trichloroethylene
Injection	: Split flow 10 mL/min 220 °C		6. 1,4-Dioxane
Detection	: FID Auto Range 220 °C		7. 4-Methyl-2-pentanone(MIBK)
Sample Size	: 2-4 ppm(V/V) in N ₂ 0.5 mL		8. Tetrachloroethylene
			9. Ethylbenzene
			10. Styrene