


## Ascorbic acid

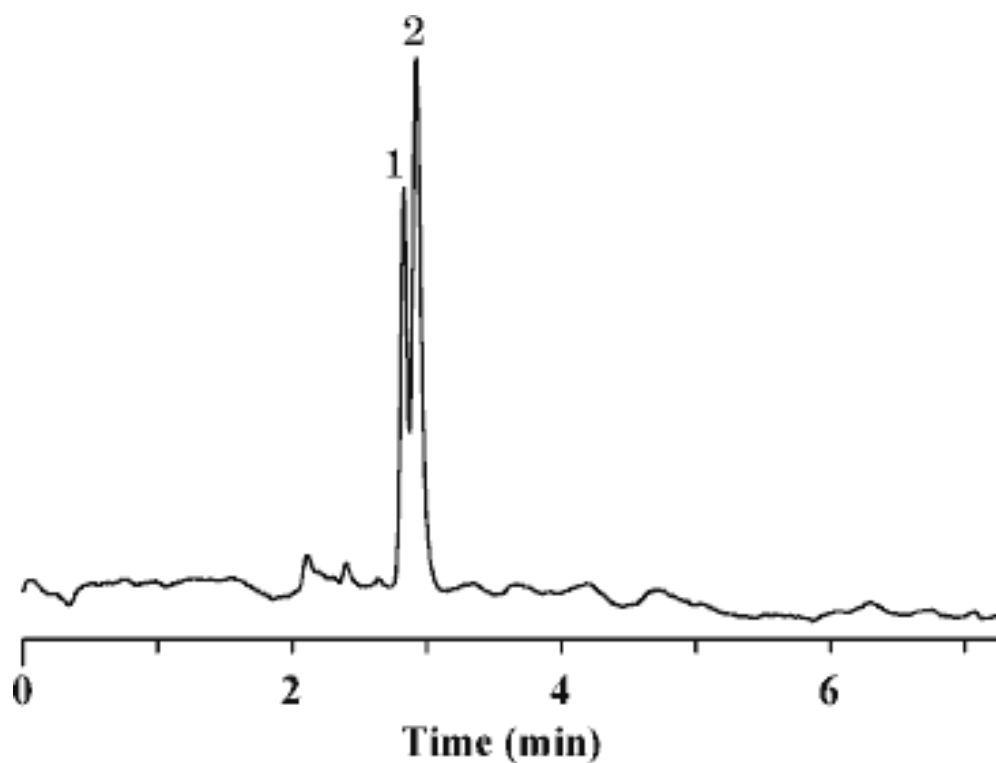

Column : Inertsil NH2

5 $\mu$ m

250  $\times$  4.6 mm I.D.

Column Cat. No. :

Eluent : 25 mM phosphate buffer (pH = 2.0)/CH<sub>3</sub>CN = 30/70

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. : 1  $\mu$ L

Sample : Ascorbic acids

Solutes : 1. D-iso-Ascorbic acid (0.05 mg/mL)

2. L-Ascorbic acid (0.05 mg/mL)