


Analysis of Carotenoids

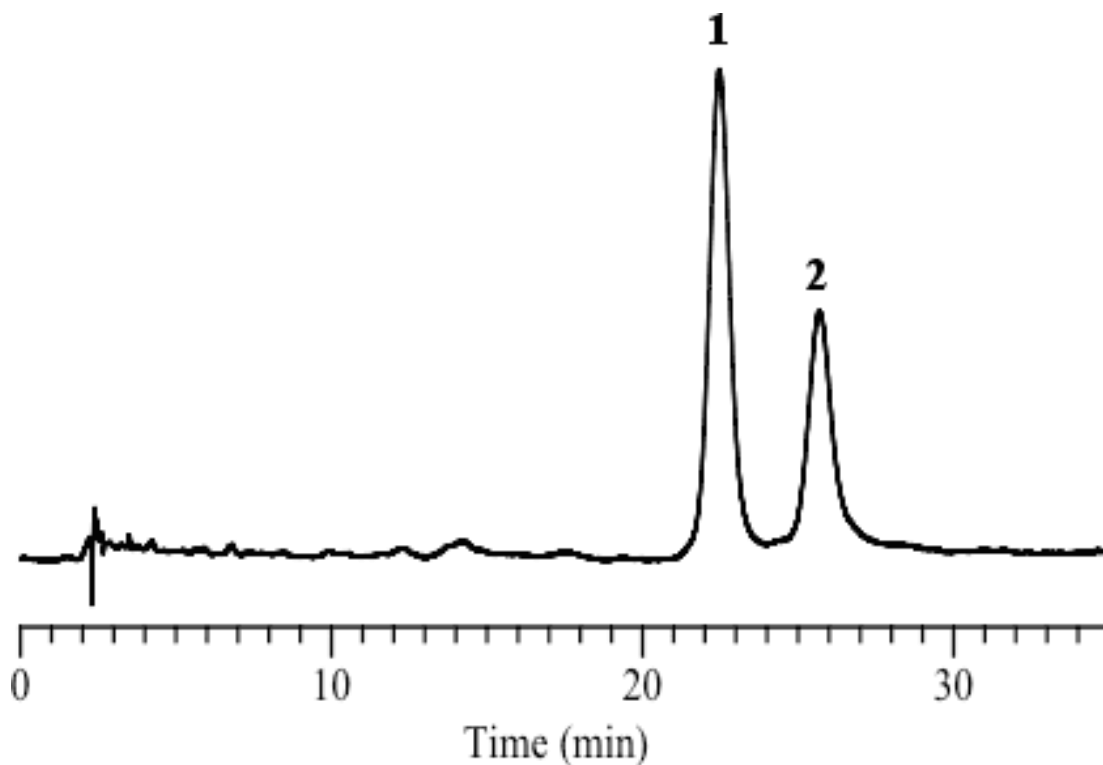

Column	:Inertsil ODS-P	Solutes	: 1. α -Carotene
	5 μ m		2. β -Carotene
	250 x 4.6 mm I.D.		

Column Cat. No.: 5020-02002

Eluent	: A) CH ₃ OH
	B) THF
	A/B = 95/5, v/v

Flow rate :1.0 mL/min.

Col. Temp. :30°C

Detection :VIS 450 nm

Injection Vol. :

Sample :