


Analysis of Carotenoids

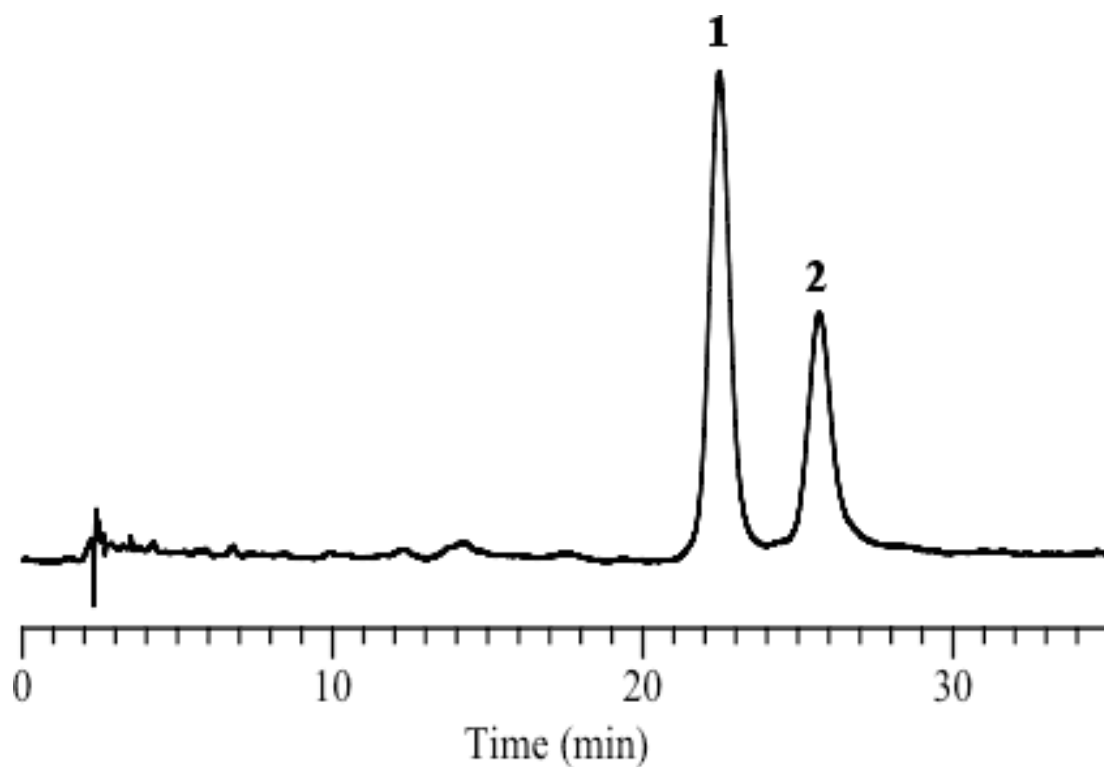

Column	:Inertsil ODS-3	Solutes	: 1. α - Carotene
	5 μ m		2. β - Carotene
	250 x 4.6 mm I.D.		

Column Cat. No.: 5020-01772

Eluent : A) CH₃OH
 B) THF
 A/B = 95/5, v/v

Flow rate :1.0 mL/min.

Col. Temp. :30°C

Detection :VIS 450 nm

Injection Vol. :

Sample :