


3. Coconut oil

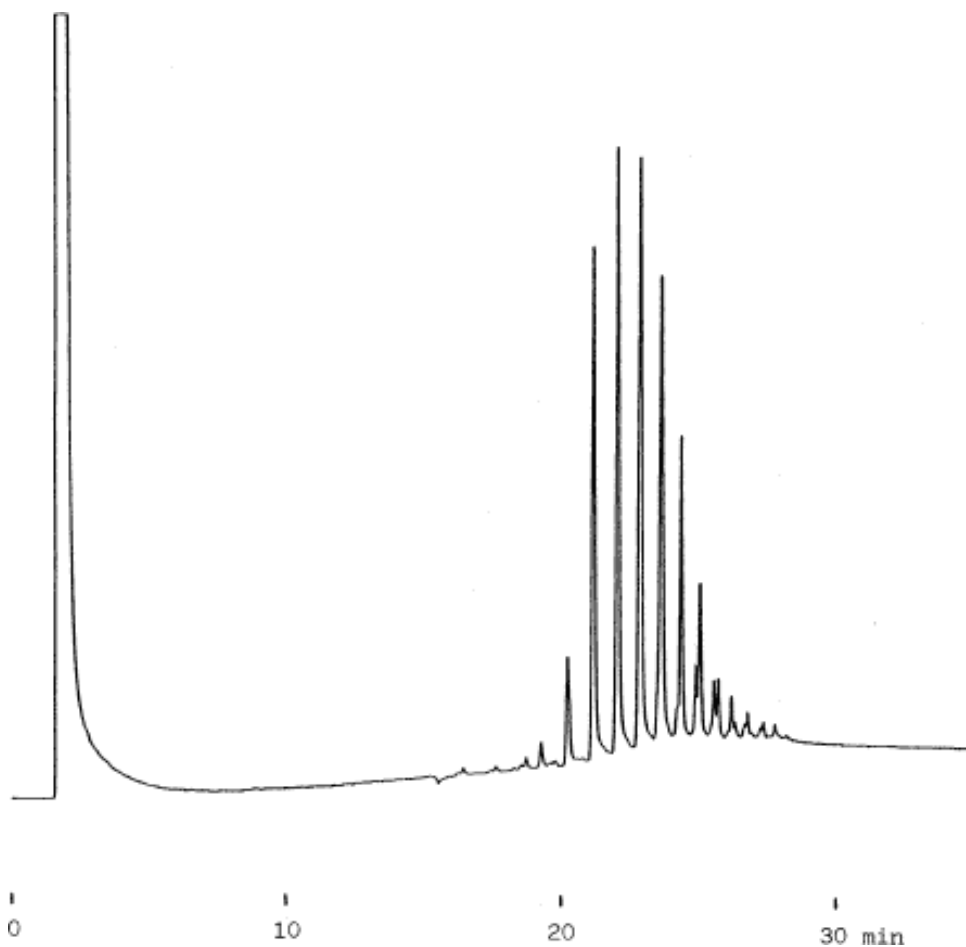

Column : Inertsil ODS-2
 5 μ m
 150 \times 0.7 mm I.D.
 Column Cat. No. : 5020-13073
 Eluent : CO₂
 Flow rate : Initial Dens.: 0.2 g/mL
 Final Dens.: 0.6 g/mL
 Program Rate: 15 μ L/min.
 Col. Temp. : 80°C
 Detection : FID 350°C
 Injection Vol. :
 Sample : Coconut Oil
 Solutes : Coconut Oil