


23. Analysis of beta-Trenbolone

Data No. LA078-0000

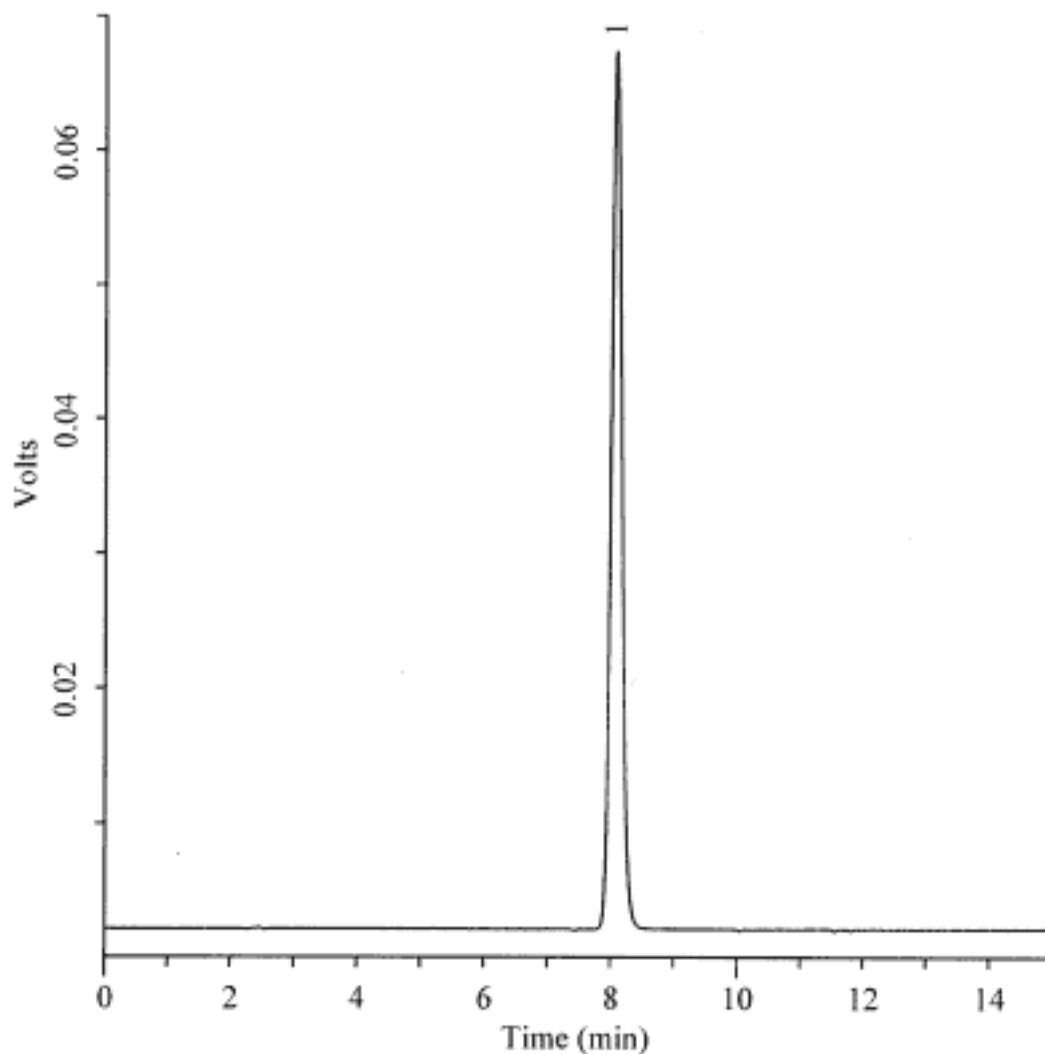

Column : Inertsil ODS-3V
150 × 4.6 mm I.D.

Column Cat. No. :

Eluent : CH₃CN/H₂O = 5/6

Flow rate : 0.6 mL/min.

Col. Temp. : 50°C

Detection : UV 340 nm

Injection Vol. : 1 µL

Sample : β-Trenbolone

Solutes : 1. β-Trenbolone (100 µg/mL)