
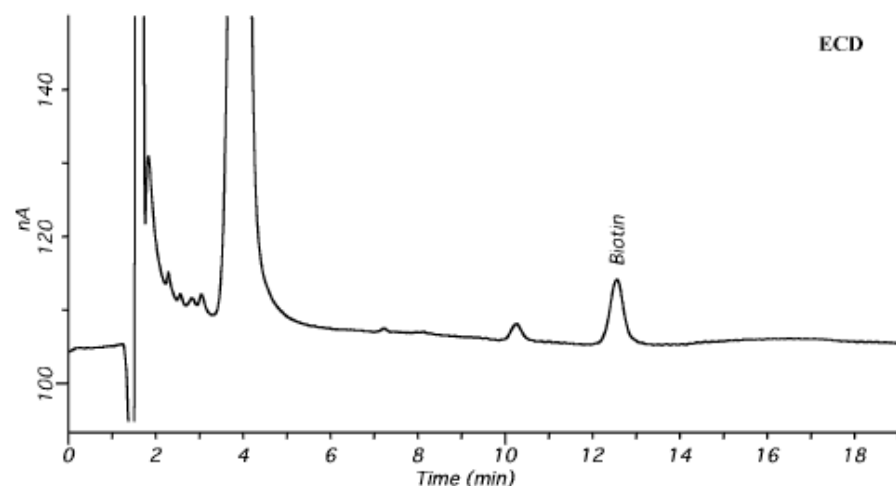


Analysis of Biotin

Data No. LA235-0000

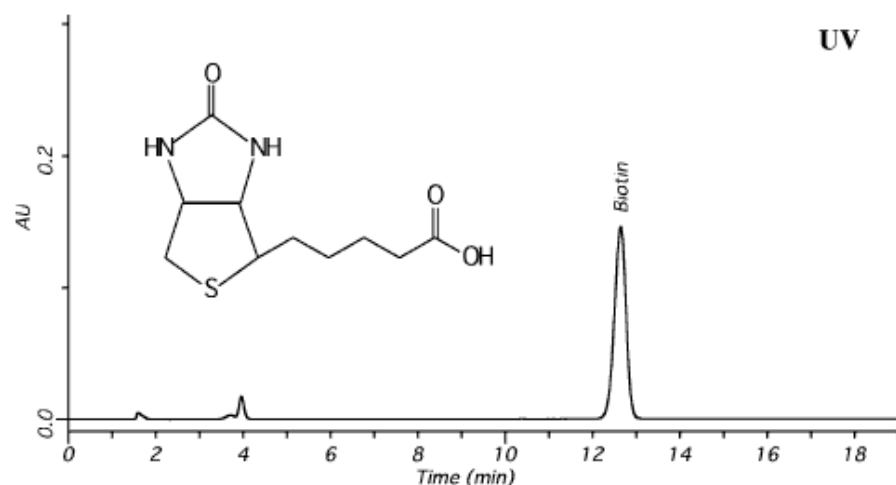

Column :Inertsil ODS-3
 5µm
 150 × 4.6mmI.D.

Column Cat. No. :

Eluent :Acetonitrile / 50 mM KH₂PO₄ (pH = 4.0 adjusted by H₃PO₄) = 10 / 90

Flow rate :1.0mL/min

Col. Temp. :40°C

Detection :UV 210 nm
 ECD 1000 mV vs. Ag / AgCl (Diamond)

Injection Vol. :10µL

Sample :1 mg / ml Biotin in 20 mM K₂HPO₄

Solutes : Biotin