


Anions

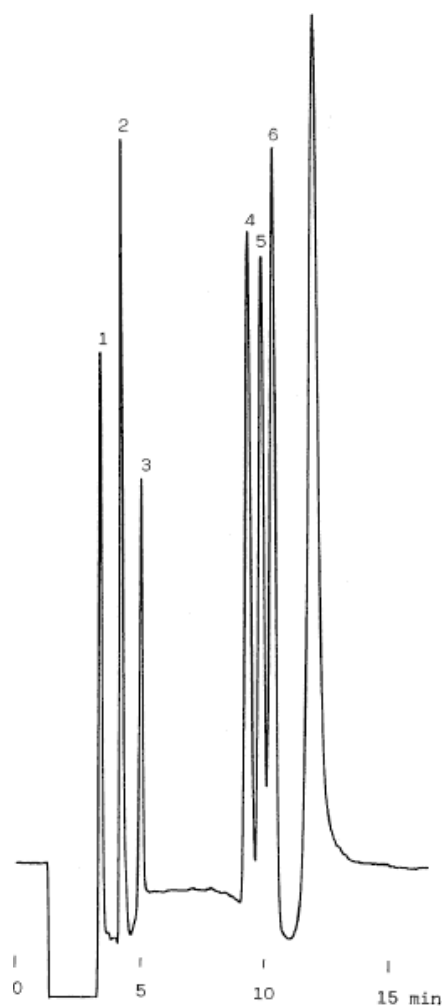

Column : Inertsil C4
5 μ m
150 \times 4.6 mm I.D.

Column Cat. No. : 5020-01401

Eluent : CH₃CN/1 mM IPCA-03H + 0.5 mM Phthalic acid =
20/80 IPCA-03H: Tetra-n-butylammonium Hydroxide

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample : Inorganic anion

Solutes : 1. CO₃²⁻
2. HPO₄²⁻
3. I⁻
4. ClO₄⁻
5. SO₄²⁻
6. S₂O₃²⁻