


Analysis of Samples for Column Selectivity

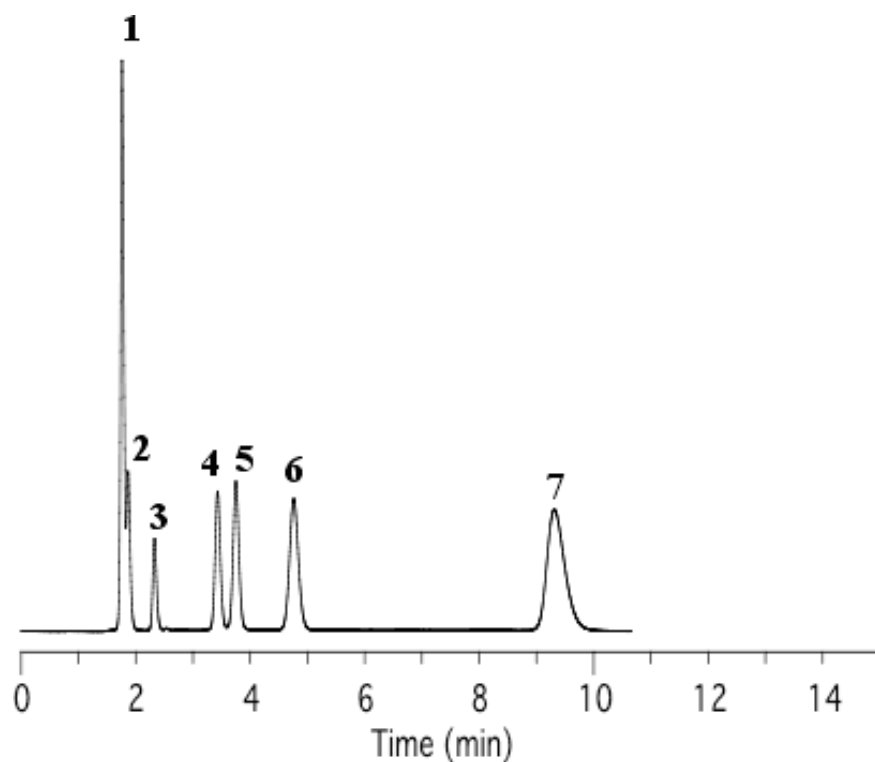

Column : Inertsil CN-3
 5 μ m
 150 x 4.6 mm I.D.

Column Cat. No. : 5020-01940

Eluent : A) CH₃OH
 B) H₂O
 A/B = 60/40, v/v

Flow rate : 1.0 mL/min.

Col. Temp. : 40°C

Detection : UV 254 nm

Injection Vol. :

Sample :

Solutes : 1. Uracil
 2. Caffeine
 3. Phenol
 4. n-Butylbenzene
 5. n-Amylbenzene
 6. o-Terphenyl
 7. Triphenylene