


Analysis of Solvents

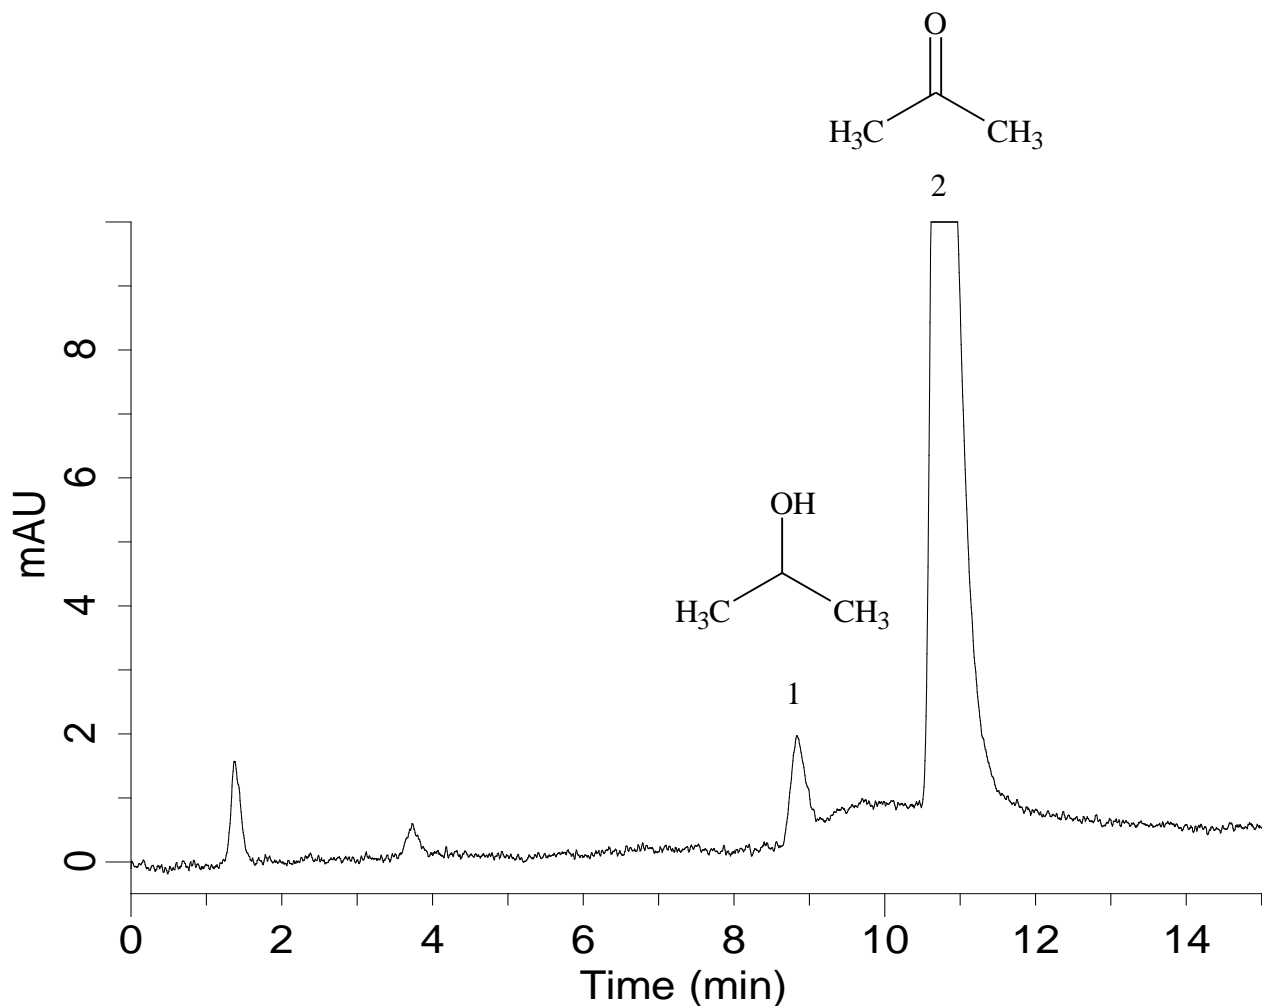

Conditions

System : GL-7400 system
Column : Inertsil ODS-SP (3 μ m, 50 x 3.0 mm I.D.)
Column Cat. No. : 5020-02822
Eluent : A) CH₃CN
 : B) H₂O
 : A/B = 2 /98 ,v/v
Flow rate : 0.4 mL/min
Col. Temp. : 20 °C
Detection : UV 190 nm (GL-7452A PDA detector)
Injection Vol. : 20 μ L

Analyte

1. 2-Propanol (100 mg/L)
 2. Acetone (100 mg/L)