


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Allantoin

Data No. LA733-0848

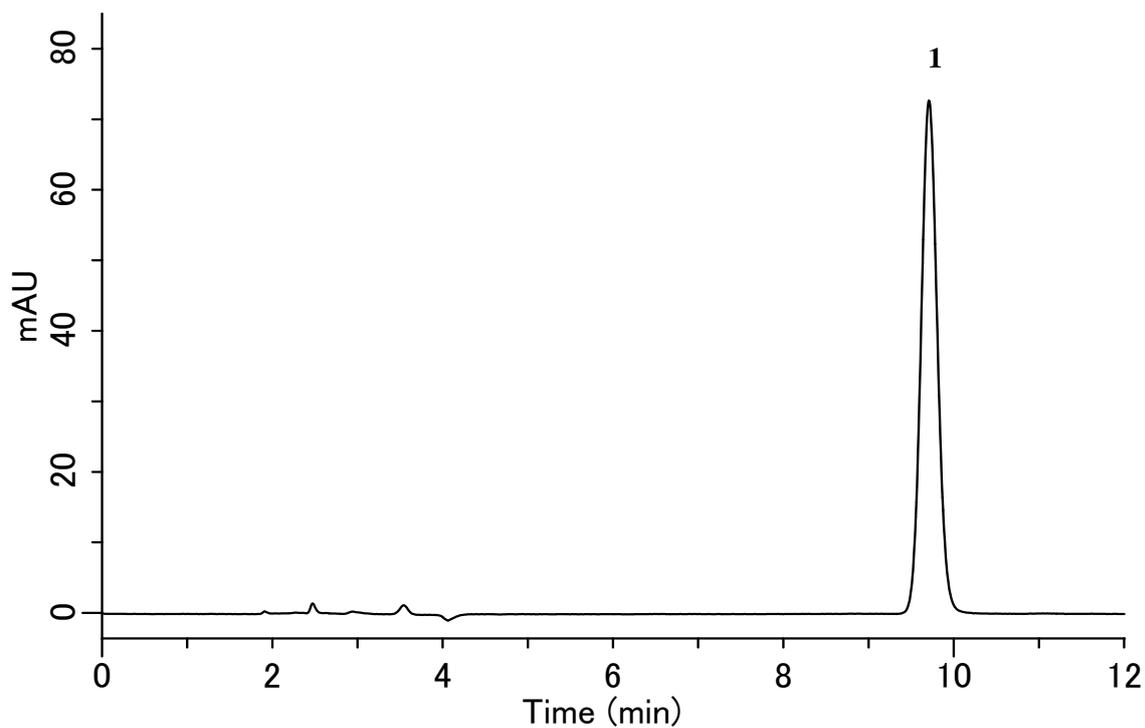

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil HILIC (5  $\mu$ m, 250 x 3.0 mm I.D.)  
**Column Cat. No.** : 5020-07716  
**Eluent** : A) CH<sub>3</sub>CN  
          : B) 10 mM CH<sub>3</sub>COONH<sub>4</sub>  
          : A/B = 95/5, v/v  
**Flow Rate** : 0.4 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 210 nm (GL-7450 UV Detector)

### Analyte

1. Allantoin