


Analysis of Allantoin

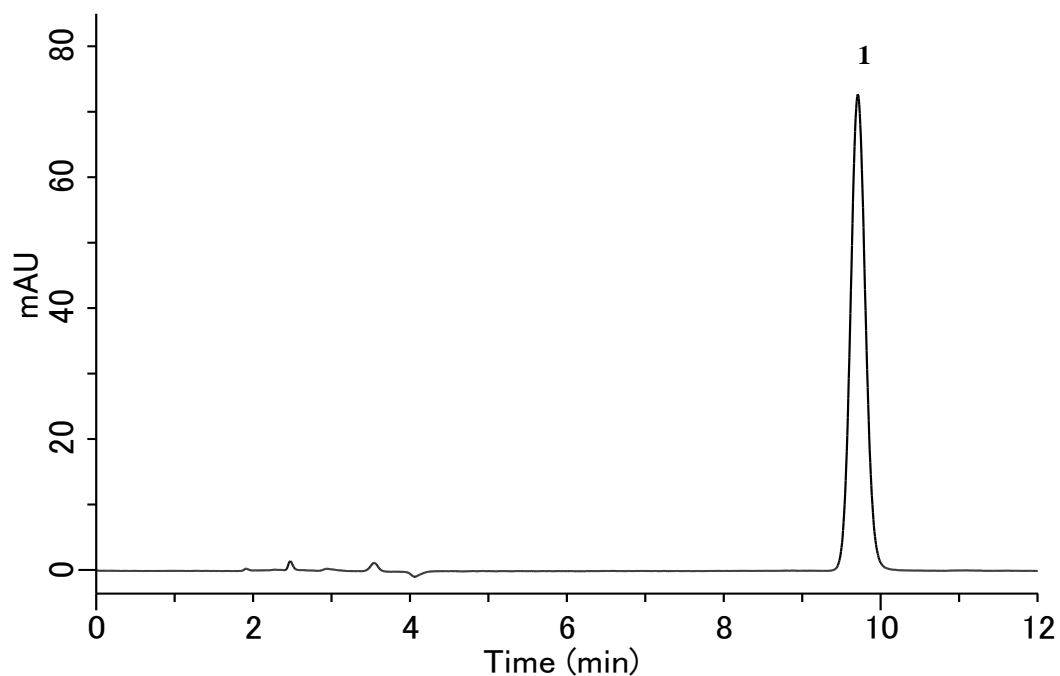

Conditions

System : GL-7400 HPLC system
Column : Inertsil HILIC (5 μ m, 250 x 3.0 mm I.D.)
Column Cat. No. : 5020-07716
Eluent : A) CH₃CN
 : B) 10 mM CH₃COONH₄
 : A/B = 95/5, v/v
Flow Rate : 0.4 mL/min
Col. Temp. : 40 °C
Detection : UV 210 nm (GL-7450 UV Detector)

Analyte

1. Allantoin