


## Analysis of Clioquinol (Inertsil ODS-4)

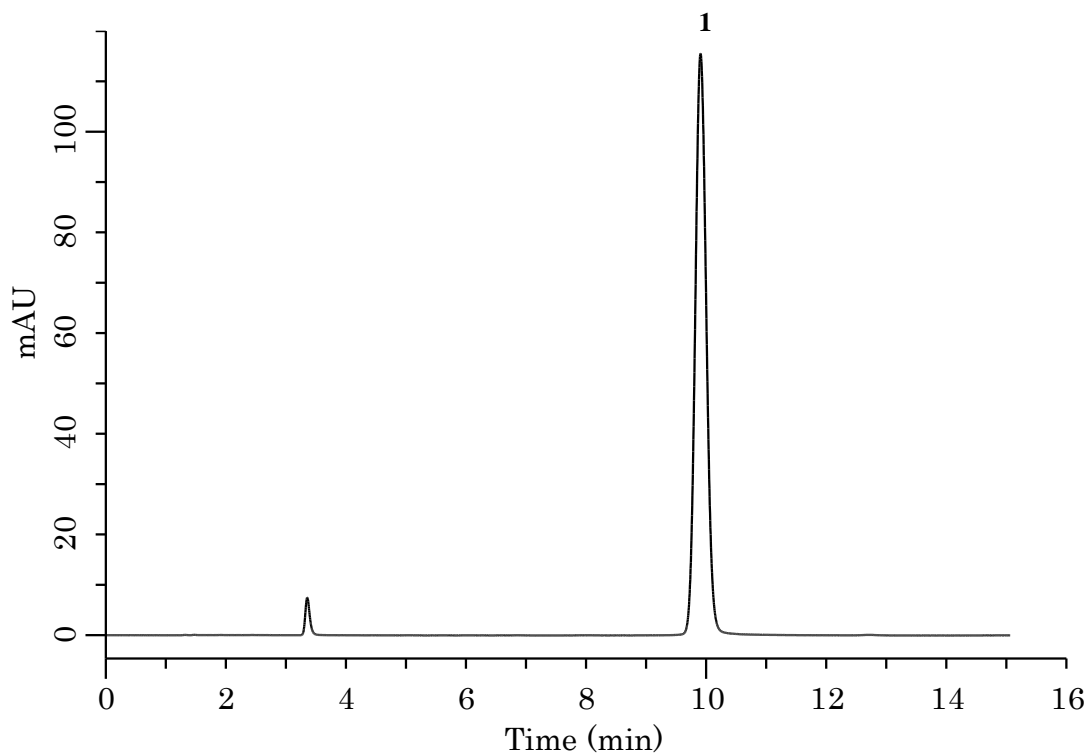

### Conditions

**System** : GL-7400 HPLC system  
**Column** : Inertsil ODS-4 (5  $\mu$ m, 150 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-03945  
**Eluent** : A) CH<sub>3</sub>CN  
          : B) 0.1 % H<sub>3</sub>PO<sub>4</sub>  
          : A/B = 60/40, v/v  
**Flow Rate** : 1 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 254 nm (GL-7450 UV Detector)  
**Injection Vol** : 2  $\mu$ L

### Analyte

1. Clioquinol (100  $\mu$ g/mL)