


InertSearch™ for LC

Inertsil® Applications

Analysis of Organic acids (Detected by Post-Column Method with BTB)

Data No. LA812-811

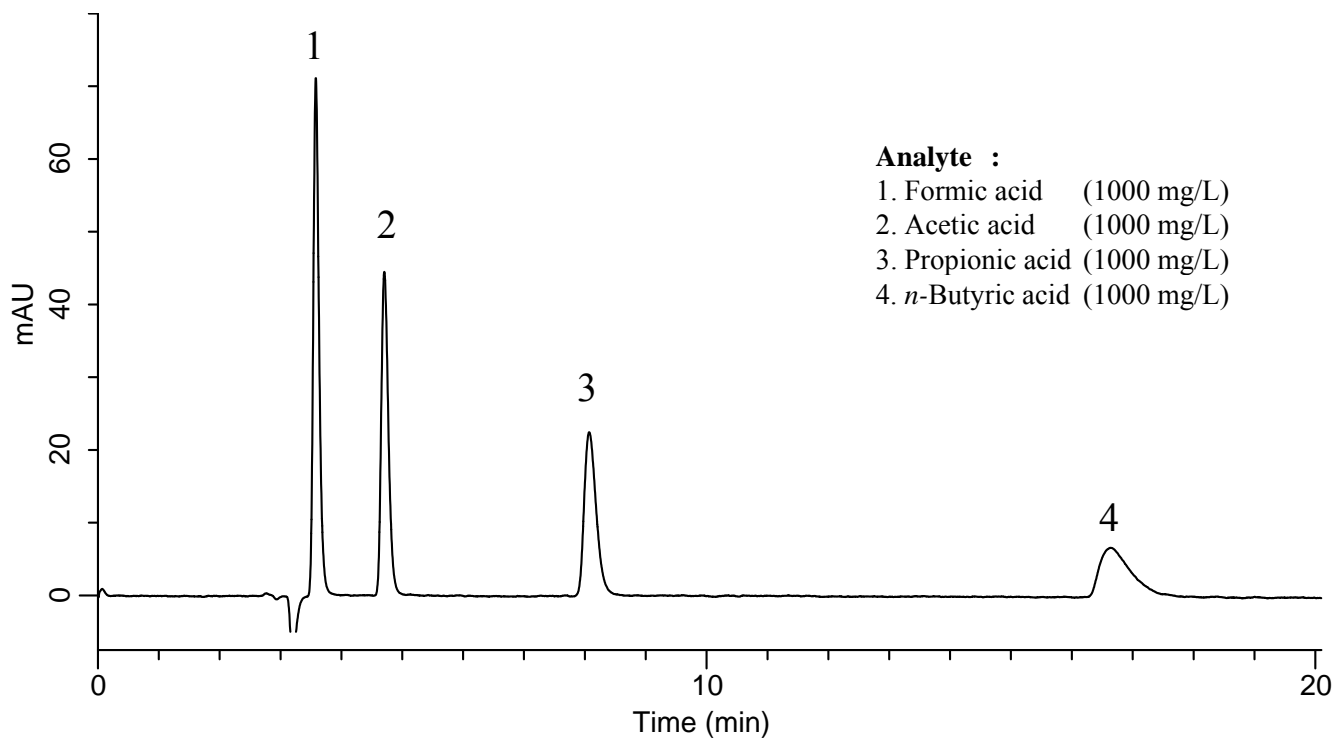

Conditions

System : GL-7400 HPLC system
Column : Inertsil Ph-3 (5 µm, 250 x 4.6 mm I.D)
Column Cat. No. : 5020-01921
Eluent : 2 mM HClO₄
Flow Rate : 1.0 mL/min
Col. Temp. : 35 °C
Detection : VIS 440 nm (GL-7450 UV Detector)
Injection Vol. : 10 µL
Sample : Organic acids