


# InertSearch™ for LC

Inertsil® Applications

## Analysis of Proteins

Data No. LA819-0699

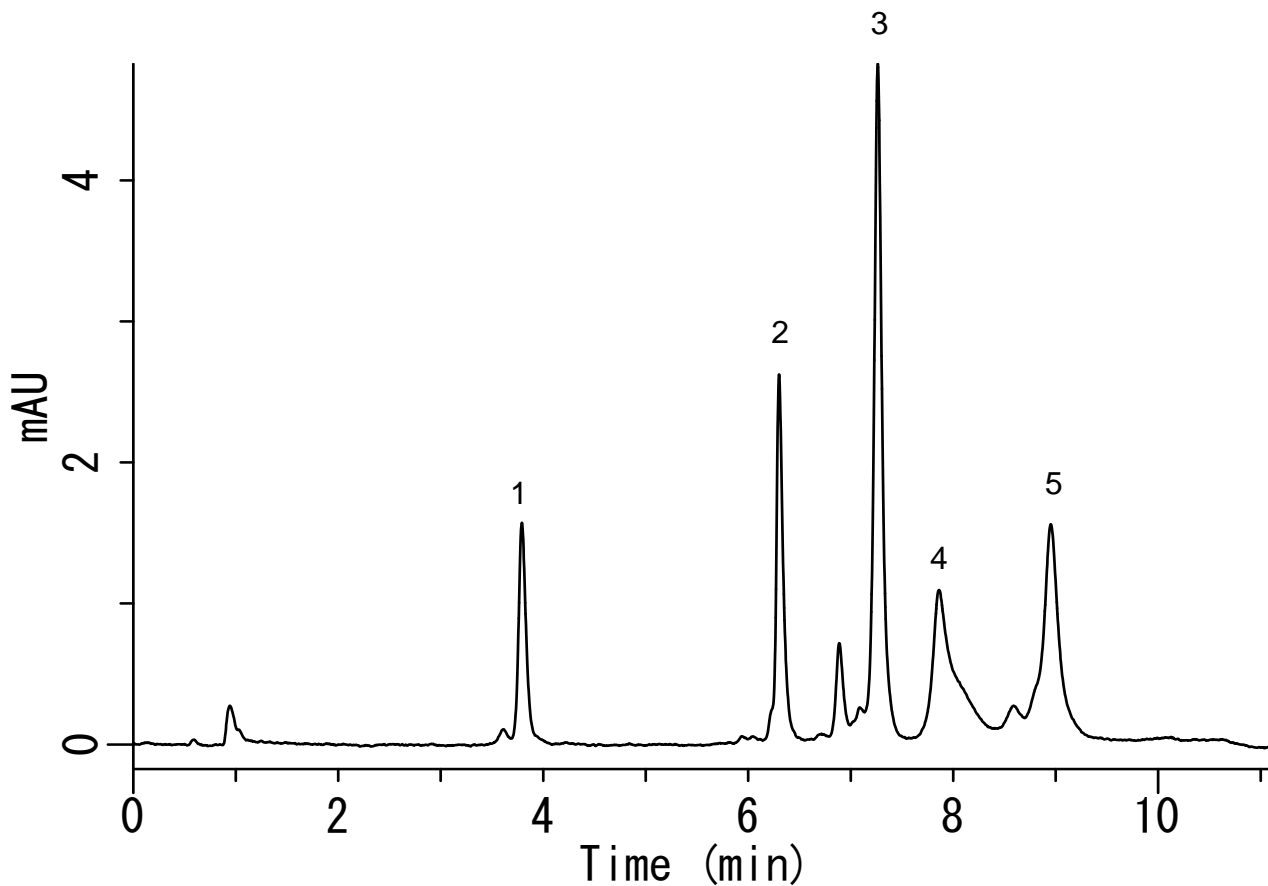

### Conditions

**System** : GL-7400 HPLC System  
**Column** : MonoClad C18-HS (150 x 3.0 mm I.D.)  
**Column Cat. No.** : 5020-10803  
**Eluent** : A) 0.1 % TFA in H<sub>2</sub>O  
          : B) 0.1 % TFA in CH<sub>3</sub>CN  
          : A/B = 75/25 – 10 min - 50/50, v/v  
**Flow Rate** : 1 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 280 nm (GL-7450 UV Detector)  
**Injection Vol.** : 1 µL

### Analyte

1. Ribonuclease A  
2. Cytochrome C  
3. Lysozyme  
4. Transferrin  
5. Conalbumin