


Analysis of Organic acids

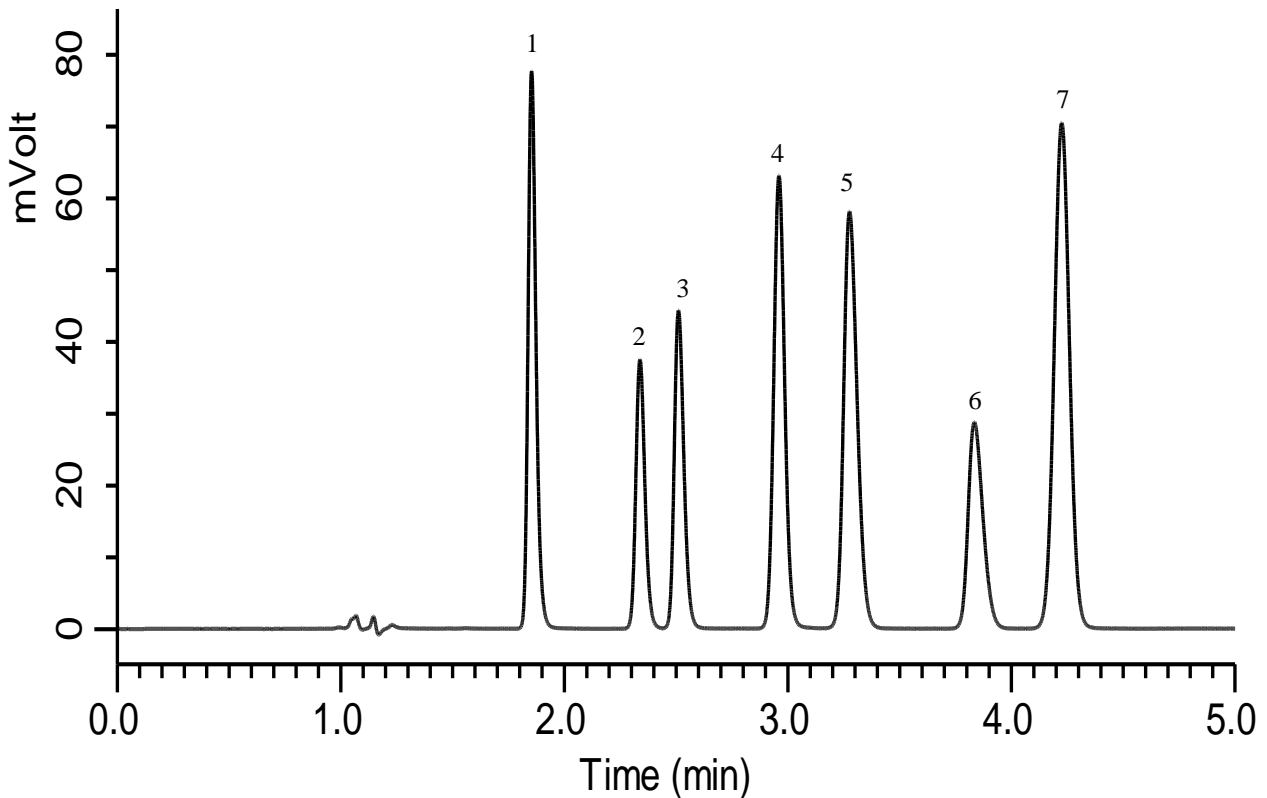

Conditions

System : LC800 HPLC system
Column : Inertsil ODS-4 (3 μ m, 150 x 3.0 mm I.D.)
Column Cat. No. : 5020-04045
Eluent : 20 mM NH₄HPO₄ (pH 2.0, H₃PO₄)
Flow Rate : 0.6 mL/min
Col. Temp. : UV 210 nm (10 mm UV cell)
Detection : 40 °C
Injection Vol. : 5 μ L
Sample : Organic acids

Analyte:

1. Malic acid	(500 mg/L)
2. Lactic acid	(500 mg/L)
3. Acetic acid	(500 mg/L)
4. Maleic acid	(5 mg/L)
5. Citric acid	(500 mg/L)
6. Succinic acid	(500 mg/L)
7. Fumaric acid	(5 mg/L)