


Analysis of Hydroquinone by HPLC-ECD

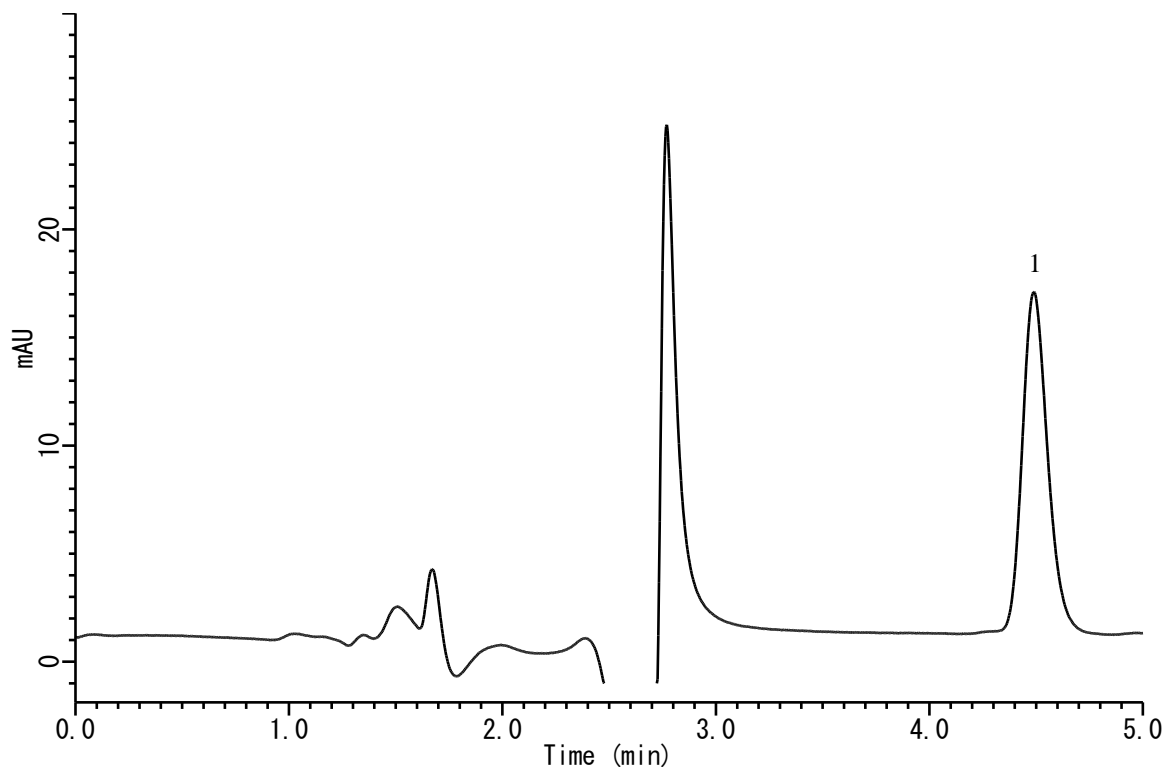

Conditions

Column : Inertsil ODS-3 (5 μ m, 150 x 3.0 mm I.D)
Column Cat. No. : 5020-01751
Eluent : A) CH₃CN
 : B) 20 mM H₃PO₄
 : A/B = 10/90, v/v
Flow Rate : 0.4 mL/min
Col. Temp. : 35 °C
Detection : ECD 1400 mV vs Ag/AgCl (ED703 EC Detector, Diamond)
Injection Vol. : 50 μ L
Sample : Standard

Analyte :

1. Hydroquinone (3 μ g/L)