



Analysis of Glutathione HPLC-ECD

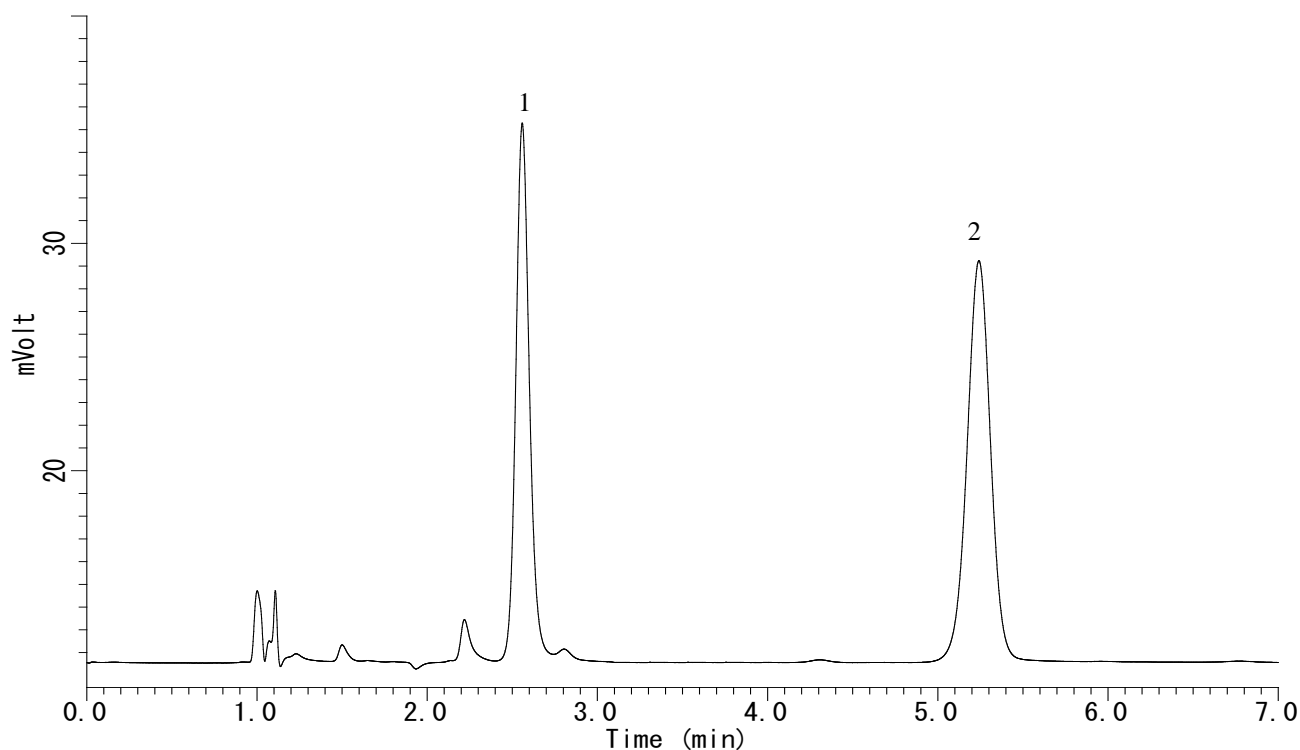

Conditions

System	: LC800 HPLC system	Analyte:	
Column	: InertSustain C18 HP (3 μ m, 150 x 3.0 mm I.D.)	1. Glutathione (GSH)	(1 μ g/mL)
Column Cat. No.	: 5020-14425	2. Glutathione Disulfide (GSSG)	(1 μ g/mL)
Eluent	: 50 mM NaH_2PO_4 (pH 2.2, H_3PO_4)		
Flow Rate	: 0.6 mL/min		
Col. Temp.	: 40 $^\circ\text{C}$		
Detection	: ECD 1200 mV vs Ag/AgCl (ED723 EC Detector, Diamond)		
Injection Vol.	: 5 μ L		
Sample	: Standard		

Analysis of Glutathione HPLC-ECD

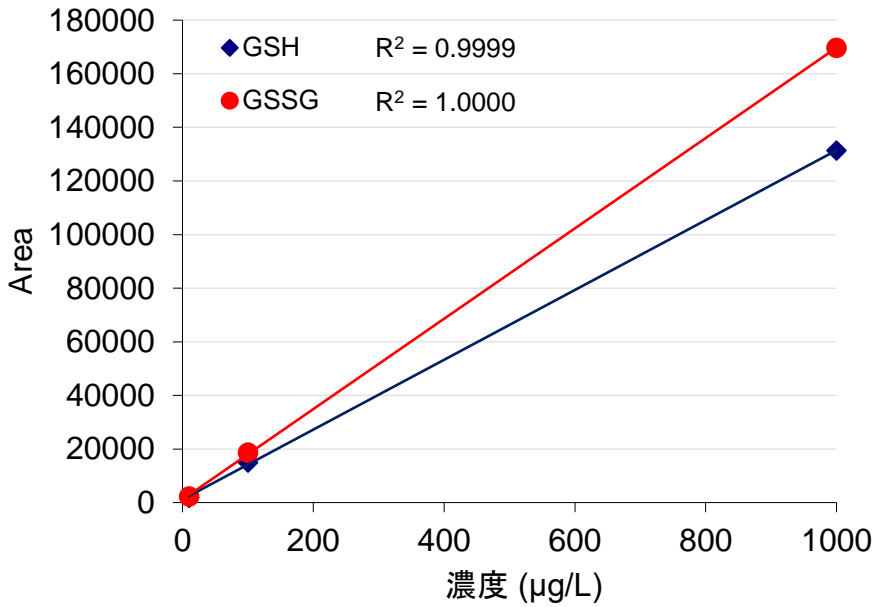

【検量線】