


InertSearch™ for LC

Inertsil® Applications

Analysis of Folic acid

Data No. LA968-0848

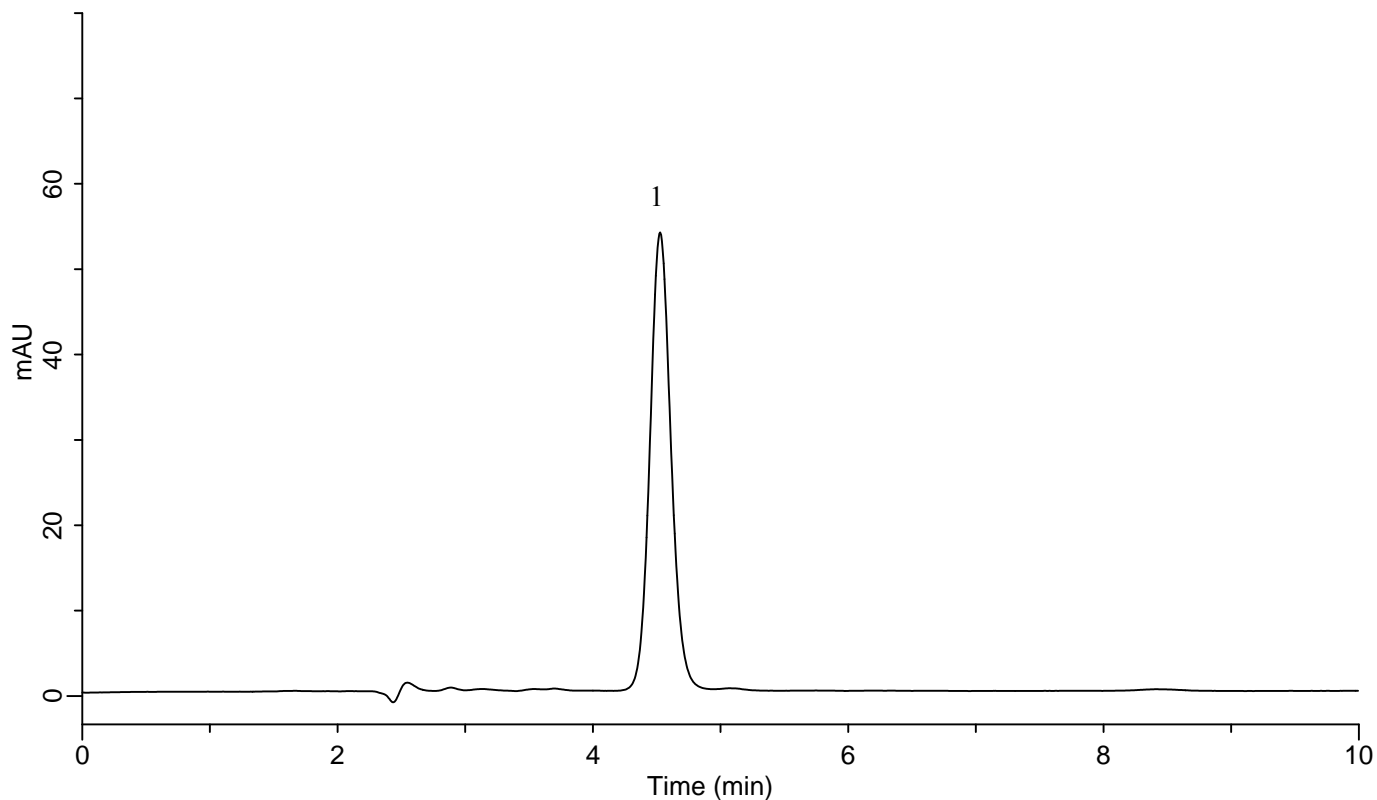

Conditions

System : LC800 HPLC System
Column : Inertsil HILIC (5 μ m, 250 x 3.0 mm I.D.)
Column Cat. No. : 5020-07716
Eluent : A) CH₃CN
 : B) 0.1 % TFA
 : A/B = 90/10 , v/v
 : (Mixed by a gradient mixer)
Flow Rate : 0.4 mL/min
Col. Temp. : 40 °C
Detection : UV 300 nm (LC800 UV Detector)
Sample : Standard

Analyte

1. Folic acid 100 mg/L