


Analysis of Antioxidant(BHT)

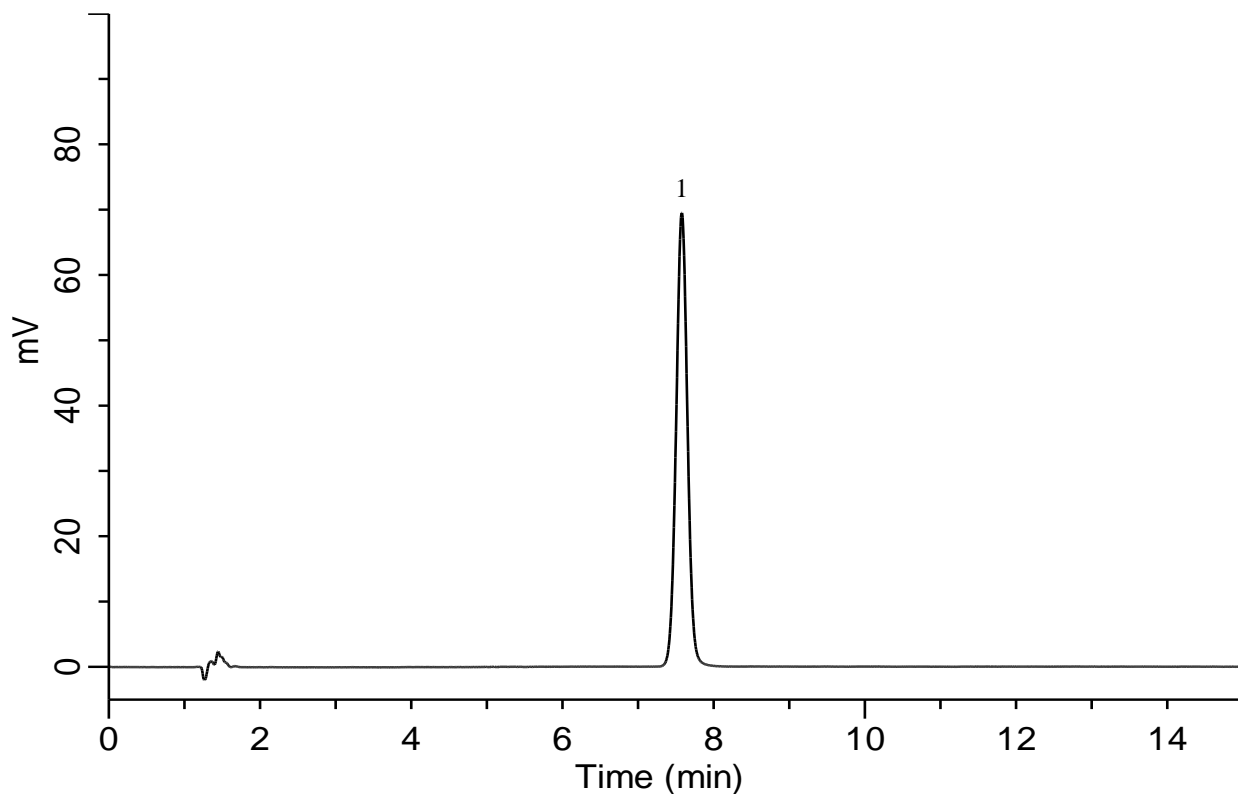

Conditions

System : LC800 HPLC System
Column : InertSustain C18 (5 μ m, 150 x 3.0 mm I.D.)
Column Cat. No. : 5020-07325
Eluent : A) CH₃CN
 B) H₂O
 A/B = 80/20, v/v
 (Mixed by a gradient mixer)
Flow Rate : 0.4 mL/min
Col. Temp. : 40 °C
Detection : UV 280 nm (LC800 UV Detector)
Injection Vol. : 10 μ L
Sample : Standard

Analyte:

1. Dibutylhydroxytoluene
 (Butylated Hydroxytoluene, BHT)
 (10 mg/L)