


InertSearch™ for LC

Inertsil® Applications

Analysis of Cyclodextrin

Data No. LB141-0642

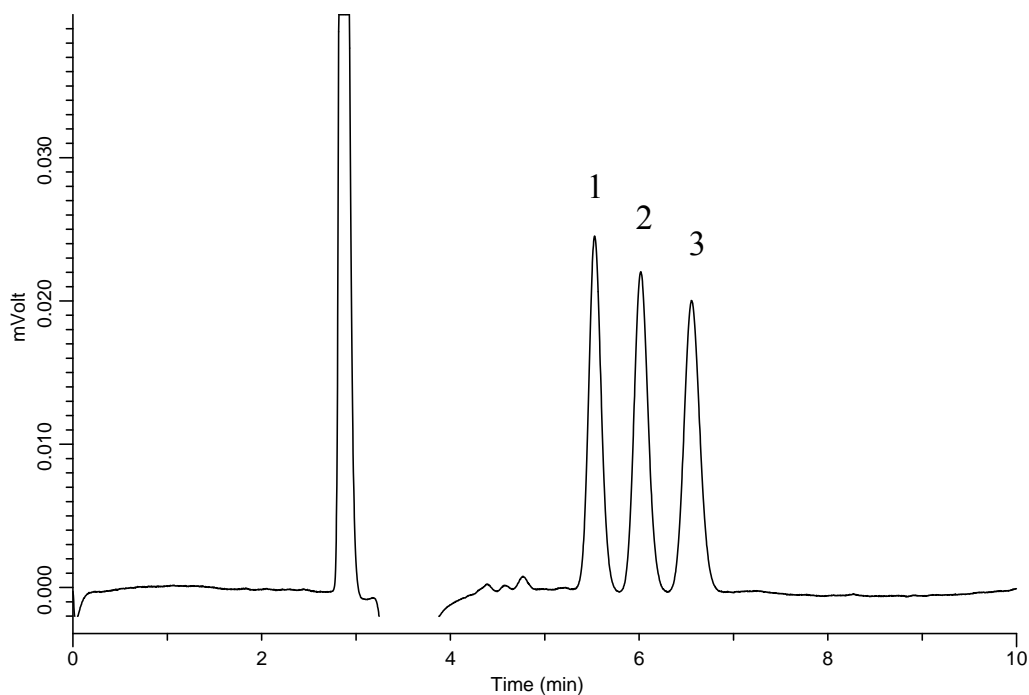

Conditions

Column : InertSustain NH₂
(5 μm, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-16628
Eluent : A) CH₃CN
B) H₂O
A/B = 60/40, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : RI
Injection Vol. : 5 μL
Sample : Standard

Analyte:

1. α-Cyclodextrin
2. β-Cyclodextrin
3. γ-Cyclodextrin