


## Analysis of Tulathromycin

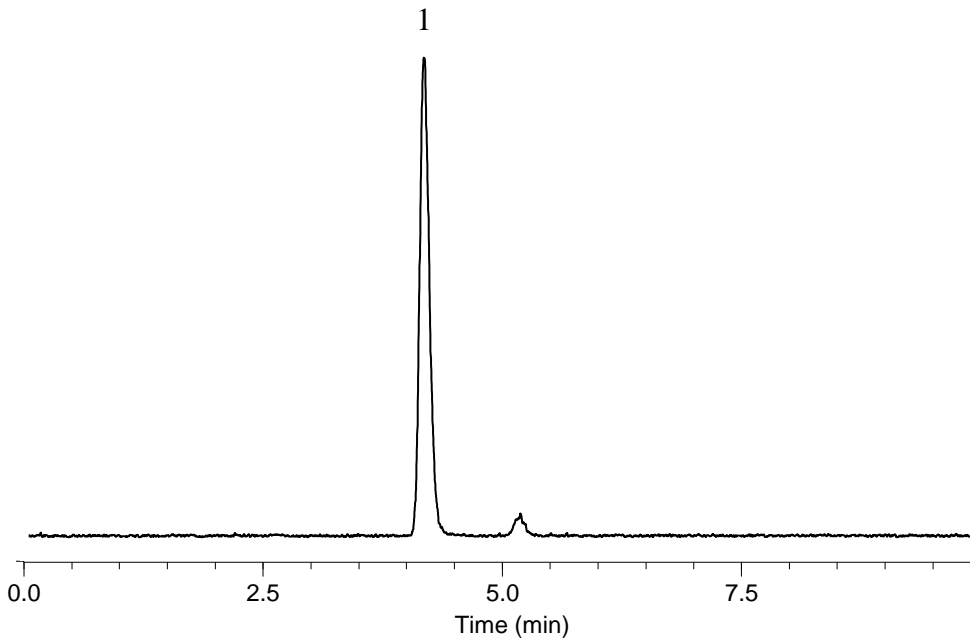

### Conditions

**Column** : InertSustainSwift C18  
 (3  $\mu$  m, 150 x 2.1 mm I.D.)  
**Column Cat. No.** : 5020-88128  
**Eluent** : A) CH<sub>3</sub>CN  
 B) 0.05 % TFA in H<sub>2</sub>O  
 A/B = 25/75, v/v  
**Flow Rate** : 0.2 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : LC/MS/MS (ESI, Positive, MRM)  
**Injection Vol.** : 1  $\mu$  L  
**Sample** : Standard

### Analyte:

1. Tulathromycin 10  $\mu$  g/L