


Analysis of Nucleoside and Nucleic acid base

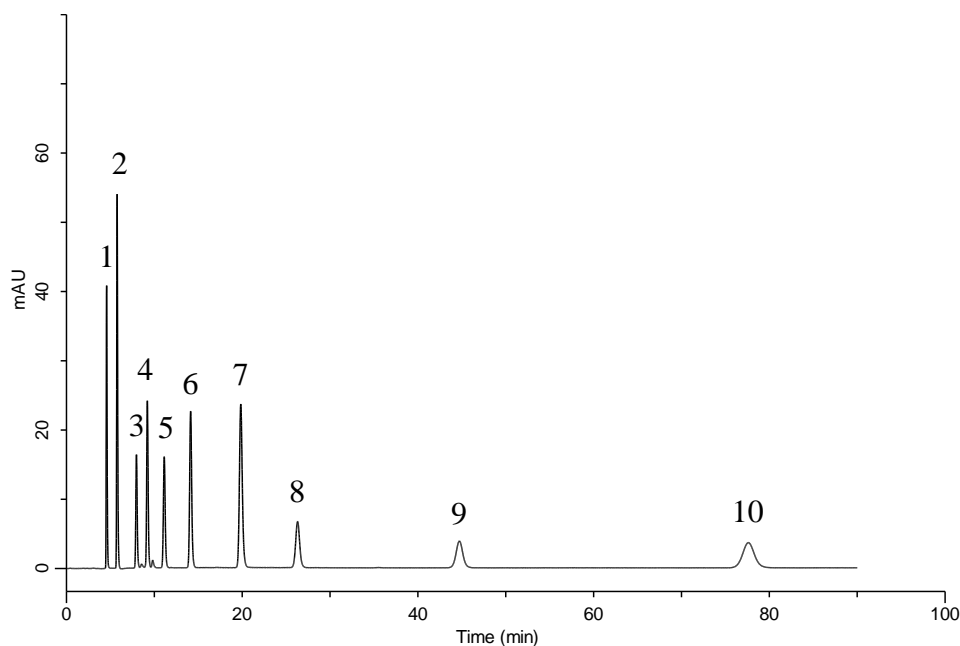

Conditions

System : GL7700 HPLC system
Column : InertSustain C18
 (5 μ m, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-07346
Eluent : 20 mM KH_2PO_4 in H_2O
 (pH7.0, 20 mM K_2HPO_4 in H_2O)
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 260 nm (PD7752 PDA Detector)
Injection Vol. : 1 μ L
Sample : Standard

Analyte:

1. Cytosine
 2. Uracil
 3. Cytidine
 4. Guanine
 5. Uridine
 6. Thymine
 7. Adenine
 8. Guanosine
 9. Thymidine
 10. Adenosine
 (100 mg/L each)