
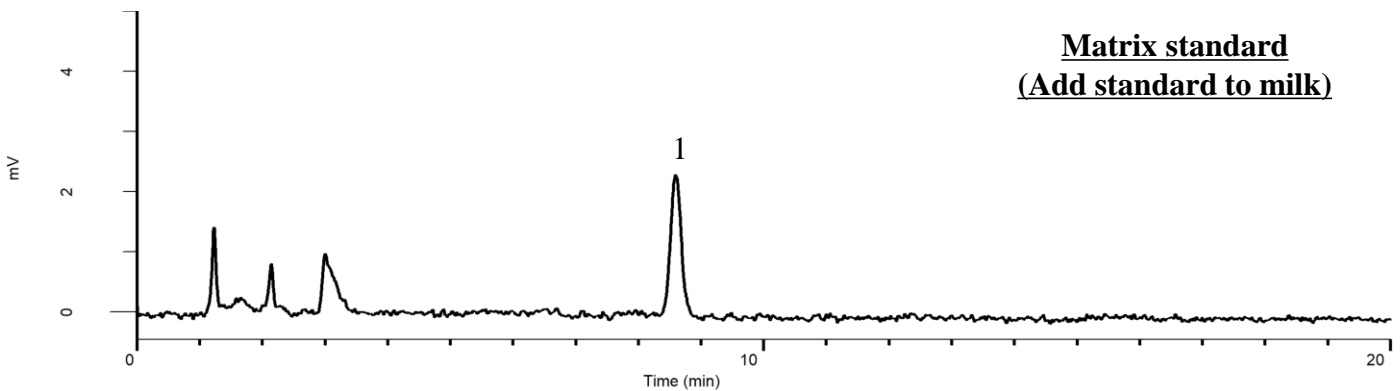


Analysis of Aflatoxin M1

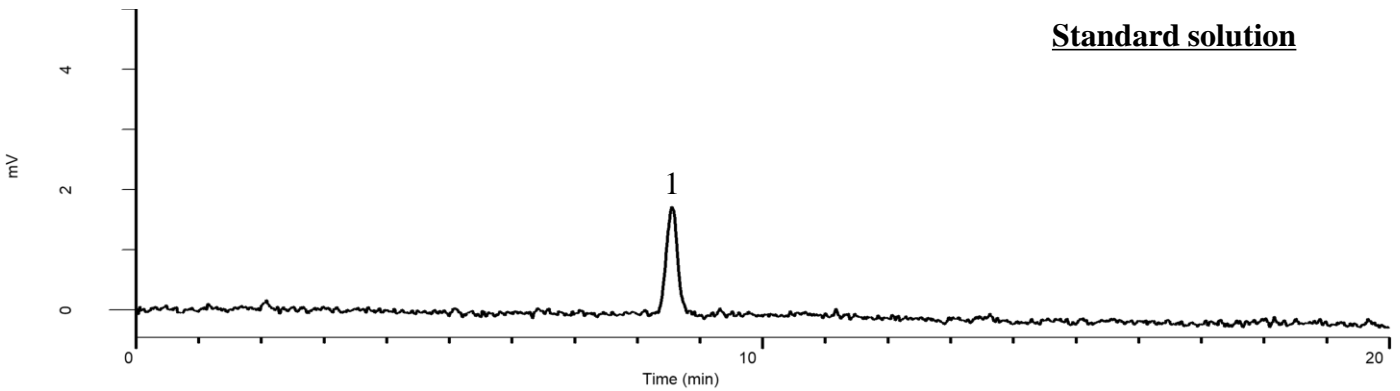

Conditions

System : GL7700 HPLC system
Column : Inertsil ODS-3
 (5 μ m, 150 x 4.6 mm I.D.)
Column Cat. No. : 5020-01731
Eluent : A) CH₃CN
 B) H₂O
 A/B = 25/75, v/v
Flow Rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 254 nm (UV7750 UV Detector)
Injection Vol. : 10 μ L

Analyte:

1. Aflatoxin M1 1 μ g / mL