


Analysis of Lactosucrose

Data No. LB479-0952

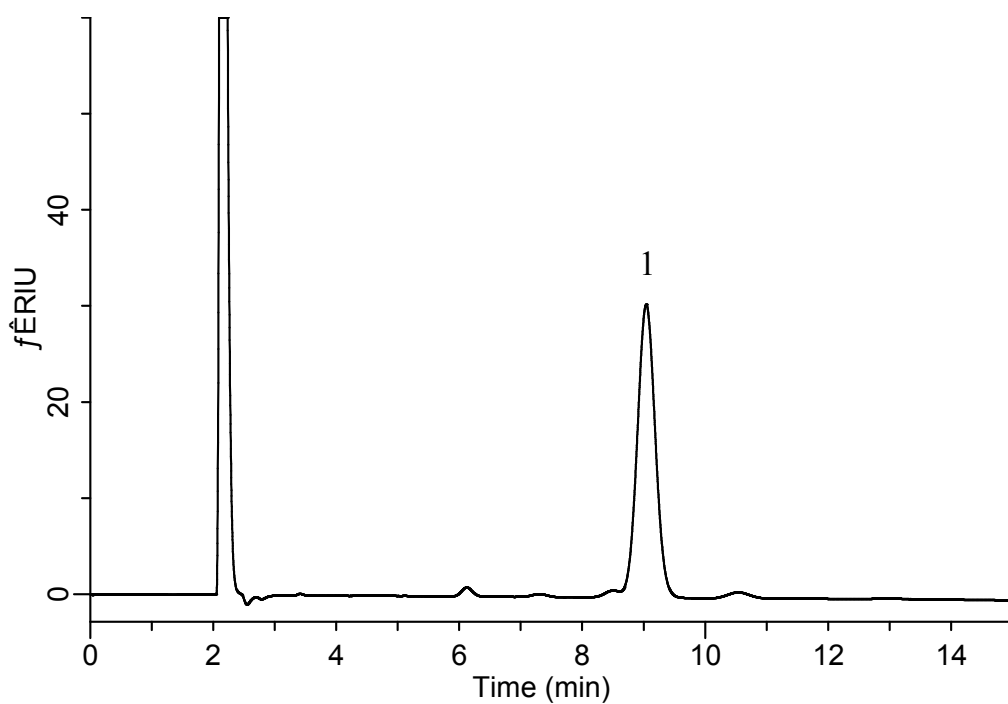

Conditions

System : GL7700 HPLC system
Column : InertSustain Amide
(5 μ m, 250 x 4.6 mm I.D.)
Column Cat. No. : 5020-88632
Eluent : A) CH₃CN
B) H₂O
A/B = 71/29, v/v
Flow Rate : 1.2 mL/min
Col. Temp. : 35 °C
Detection : RI (RI7754 RI Detector)
Injection Vol. : 20 μ L
Sample : Standard

Analyte:

1. Lactosucrose 5.0 mg/mL
(Dissolved in CH₃CN/H₂O = 50/50)