


## Analysis of Etoposide phosphate

(Under the Condition of draft for USP)

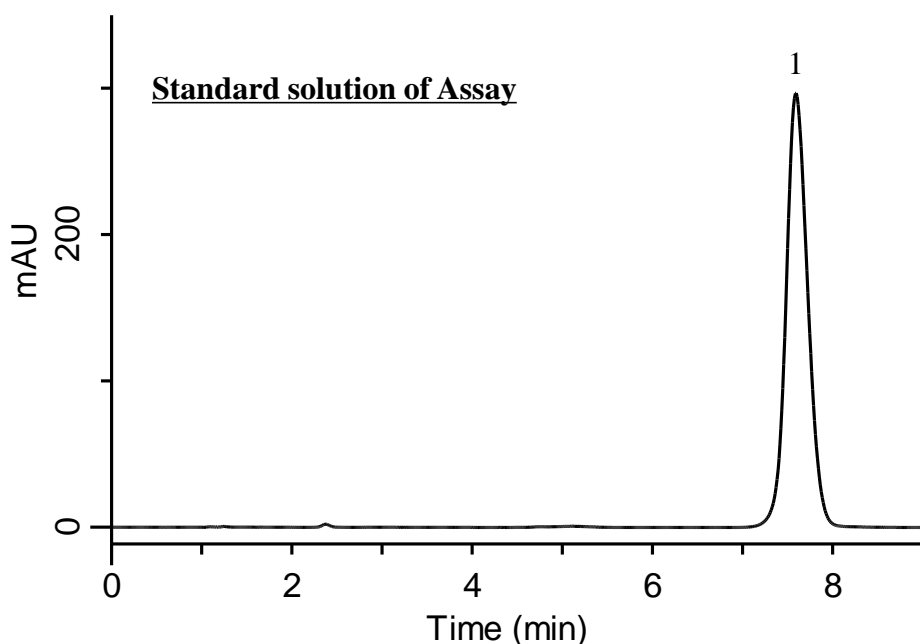

### Conditions

**System** : GL7700 HPLC system  
**Column** : InertSustain Phenyl  
 (5  $\mu$  m, 150 x 4.6 mm I.D.)  
**Column Cat. No.** : 5020-16327  
**Eluent** : A) CH<sub>3</sub>CN  
 B) SolutionA\*  
 A/B = 15/85, v/v\*\*  
**Flow Rate** : 1.5 mL/min  
**Col. Temp.** : 40 °C  
**Detection** : UV 230 nm (PD7752 PDA Detector)  
**Injection Vol.** : 25  $\mu$  L  
**Sample** : Standard

### Analyte:

1. Etoposide phosphate 0.24 mg/mL

Symmetry factor : 1.10 ( $\leq$  1.5)  
 RSD of the peak area %(n=6) : 0.17 ( $\leq$  0.73)

\* 2.3g/L of ammonium phosphate, monobasic in water.

\*\* Acetonitrile and SolutionA (15 : 85). Adjust with phosphoric acid to a pH 2.5.