


Analysis of Stearyl Glycyrrhetinate

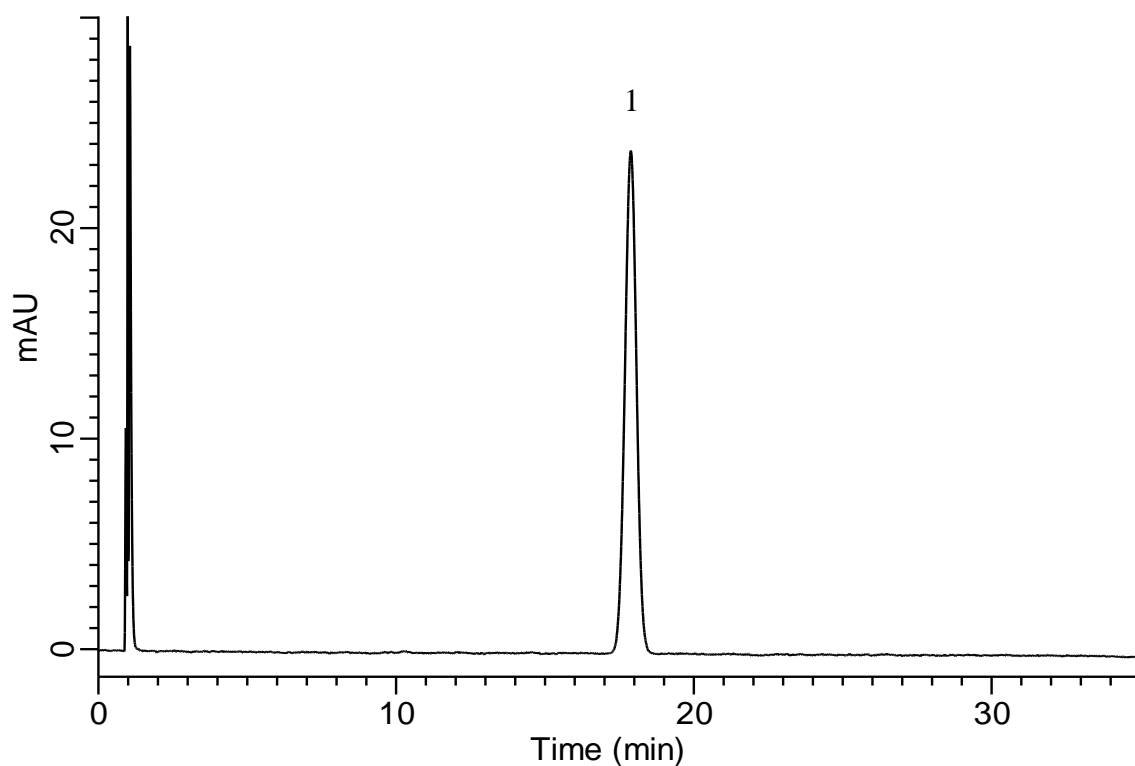

Conditions

System : Chromaster
Column : InertSustainSwift C8
 (3 μ m, 3.0 x 100 mmI.D.)
Column Cat. No. : 5020-88437
Eluent : A) CH₃CN
 B) H₂O
 A/B = 85/15, v/v
Flow Rate : 0.6 mL/min
Col. Temp. : 40 °C
Detection : UV 250 nm (5430 Diode Array Detector)
Injection Vol. : 5 μ L
Sample : Standard

Analyte:

1. Stearyl Glycyrrhetinate 100 mg/L