


InertSearch for LC

Inertsil Applications

Analysis of Coenzyme A (CoA)

Data No. LB778-0806

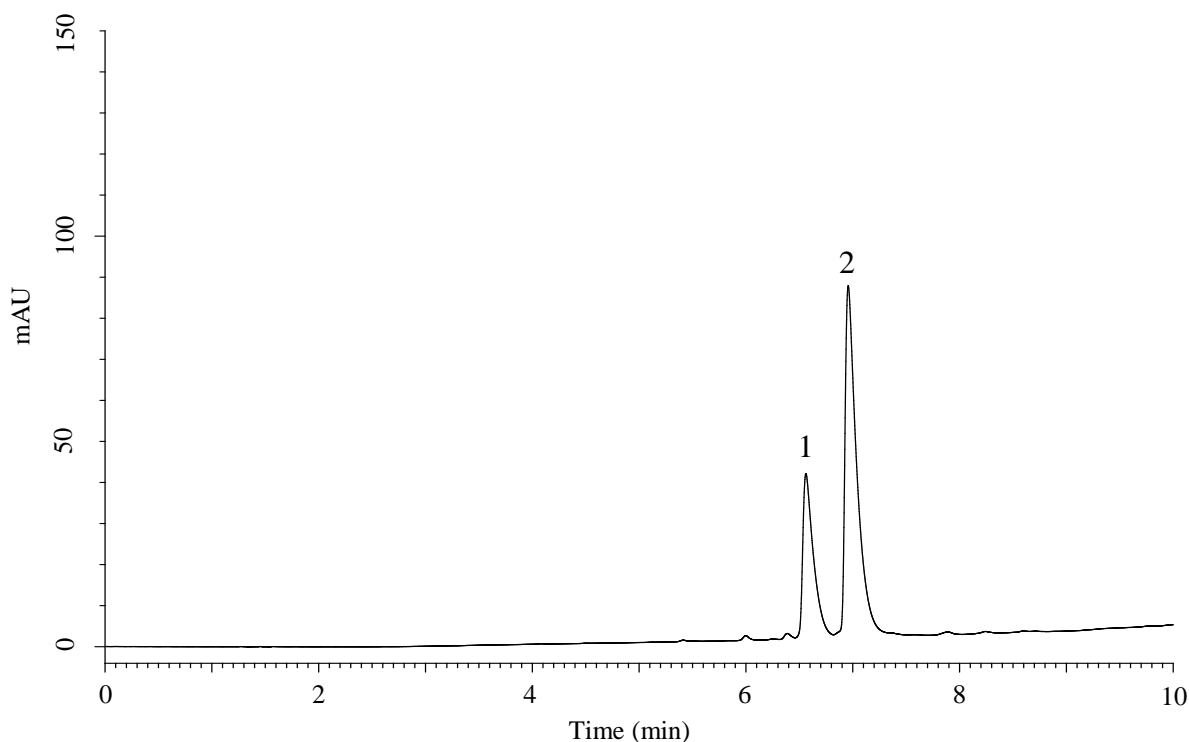

Conditions

Column : InertSustain AX-C18 (GL Sciences Inc.)
(3 μ m, 150 x 2.1 mm I.D., Metal-free hardware)

Column Cat. No. : 5020-91059

Eluent : A) 200 mM HCOONH₄ in CH₃OH
B) 10 mM HCOONH₄ in H₂O

Analyte:

1. Coenzyme A
2. Acetyl coenzyme A
(100 mg/L each)

Time (min)	A (vol%)	B (vol%)
0.0	5	95
10.0	100	0

Flow Rate : 0.3 mL/min
Col. Temp. : 40 °C
Detection : UV 254 nm
Injection Vol. : 1 μ L
Sample : Standard